

RESEARCH ARTICLE

# Recalibration of the Limiting Antigen Avidity EIA to Determine Mean Duration of Recent Infection in Divergent HIV-1 Subtypes

Yen T. Duong<sup>1</sup>, Reshma Kassanjee<sup>3,4</sup>, Alex Welte<sup>3</sup>, Meade Morgan<sup>2</sup>, Anindya De<sup>2</sup>, Trudy Dobbs<sup>1</sup>, Erin Rottinghaus<sup>1</sup>, John Nkengasong<sup>1</sup>, Marcel E. Curlin<sup>5</sup>, Chonticha Kittinunvorakoon<sup>5</sup>, Boonyos Raengsakulrach<sup>5</sup>, Michael Martin<sup>5</sup>, Kachit Choopanya<sup>5</sup>, Suphak Vanichseni<sup>5</sup>, Yan Jiang<sup>6</sup>, Maofeng Qiu<sup>6</sup>, Haiying Yu<sup>6</sup>, Yan Hao<sup>6</sup>, Neha Shah<sup>7</sup>, Linh-Vi Le<sup>8</sup>, Andrea A. Kim<sup>9</sup>, Tuan Anh Nguyen<sup>10</sup>, William Ampofo<sup>11</sup>, Bharat S. Parekh<sup>1\*</sup>



CrossMark  
click for updates

OPEN ACCESS

**Citation:** Duong YT, Kassanjee R, Welte A, Morgan M, De A, Dobbs T, et al. (2015) Recalibration of the Limiting Antigen Avidity EIA to Determine Mean Duration of Recent Infection in Divergent HIV-1 Subtypes. PLoS ONE 10(2): e0114947. doi:10.1371/journal.pone.0114947

**Academic Editor:** Francesca Ceccherini-Silberstein, University of Rome Tor Vergata, ITALY

**Received:** July 31, 2014

**Accepted:** November 16, 2014

**Published:** February 24, 2015

**Copyright:** This is an open access article, free of all copyright, and may be freely reproduced, distributed, transmitted, modified, built upon, or otherwise used by anyone for any lawful purpose. The work is made available under the [Creative Commons CC0](https://creativecommons.org/licenses/by/4.0/) public domain dedication.

**Data Availability Statement:** All relevant data are within the paper and its Supporting Information files.

**Funding:** This research has been supported by the President's Emergency Plan for AIDS Relief (PEPFAR) through the Centers for Disease Control and Prevention (CDC). The findings and conclusions in this report are those of the authors and do not necessarily represent the official position of the CDC/ Agency for Toxic Substances and Disease Registry. AW and RK are grateful for support from the Bill and Melinda Gates Foundation through (and to their colleagues at) the Consortium for the Evaluation and

**1** International Laboratory Branch, Division of Global HIV/AIDS, Centers for Disease Control and Prevention, Atlanta, Georgia, United States of America, **2** Epidemiology and Strategic Information Branch, Division of Global HIV/AIDS, Centers for Disease Control and Prevention, Atlanta, Georgia, United States of America, **3** The South African DST/NRF Centre of Excellence in Epidemiological Modelling and Analysis (SACEMA), University of Stellenbosch, Stellenbosch, South Africa, **4** School of Computational and Applied Mathematics, University of the Witwatersrand, Johannesburg, South Africa, **5** Thailand Ministry of Public Health-US CDC Collaboration, Bangkok, Thailand, **6** National AIDS Reference Laboratory, National Center for AIDS/STD Control and Prevention, Chinese Center for Disease Control and Prevention, Beijing, China, **7** California Department of Public Health, Richmond, California, United States of America, **8** Division of Global HIV/AIDS, Centers for Disease Control and Prevention, Hanoi, Vietnam, **9** CDC-Kenya, Nairobi, Kenya, **10** National Institute of Hygiene and Epidemiology, Hanoi, Vietnam, **11** Noguchi Memorial Institute for Medical Research, Accra, Ghana

\* [bparekh@cdc.gov](mailto:bparekh@cdc.gov)

## Abstract

### Background

Mean duration of recent infection (MDRI) and misclassification of long-term HIV-1 infections, as proportion false recent (PFR), are critical parameters for laboratory-based assays for estimating HIV-1 incidence. Recent review of the data by us and others indicated that MDRI of LAg-Avidity EIA estimated previously required recalibration. We present here results of recalibration efforts using >250 seroconversion panels and multiple statistical methods to ensure accuracy and consensus.

### Methods

A total of 2737 longitudinal specimens collected from 259 seroconverting individuals infected with diverse HIV-1 subtypes were tested with the LAg-Avidity EIA as previously described. Data were analyzed for determination of MDRI at ODn cutoffs of 1.0 to 2.0 using 7 statistical approaches and sub-analyzed by HIV-1 subtypes. In addition, 3740 specimens from individuals with infection >1 year, including 488 from patients with AIDS, were tested for PFR at varying cutoffs.

Performance of HIV Incidence Assays, and the HIV Modeling Consortium. The funders had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript.

**Competing Interests:** BSP is an inventor of LAg-Avidity EIA and receives royalties as part of U.S. government licensing agreement with commercial partners. Recombinant protein (rIDRm) and knowhow to develop the LAg-Avidity EIA and related incidence assays have been licensed to multiple commercial partners as per open licensing policy of the U.S. Government. These commercial partners currently include 1) Sedia BioSciences, Portland, OR, 2) Maxim Biotech, Rockville, MD, and 3) Beijing KingHawk Pharmaceuticals Inc., Beijing, China. This does not alter the authors' adherence to PLOS ONE Editorial policies and criteria or adherence of PLOS ONE policies on sharing data and materials.

## Results

Using different statistical methods, MDRI values ranged from 88–94 days at cutoff  $OD_n = 1.0$  to 177–183 days at  $OD_n = 2.0$ . The MDRI values were similar by different methods suggesting coherence of different approaches. Testing for misclassification among long-term infections indicated that overall PFRs were 0.6% to 2.5% at increasing cutoffs of 1.0 to 2.0, respectively. Balancing the need for a longer MDRI and smaller PFR (<2.0%) suggests that a cutoff  $OD_n = 1.5$ , corresponding to an MDRI of 130 days should be used for cross-sectional application. The MDRI varied among subtypes from 109 days (subtype A&D) to 152 days (subtype C).

## Conclusions

Based on the new data and revised analysis, we recommend an  $OD_n$  cutoff = 1.5 to classify recent and long-term infections, corresponding to an MDRI of 130 days (118–142). Determination of revised parameters for estimation of HIV-1 incidence should facilitate application of the LAg-Avidity EIA for worldwide use.

## Introduction

Laboratory methods to detect recent HIV infection and estimate HIV incidence using cross-sectional specimens continues to be a high priority because they have the potential to help monitor the leading edge of the epidemic, target resources and evaluate successes of prevention programs in a very cost-effective and timely manner [1–18]. Measurement of HIV-1 incidence is also critical for identifying high incidence populations for prevention trials, including efficacy of candidate vaccines and other interventions.

The development of an optimal laboratory method for worldwide use has remained challenging due to the diversity of HIV-1 subtypes, biologic differences among populations or limitation of the assays [1,19–25]. Several reviews and reports have been written summarizing the status of the evolving research in this area; they have stressed the need for accurate calibration of assays or algorithms but substantive progress has been slow [4,22,26–31].

In the absence of reliable laboratory methods, UNAIDS and others have derived incidence estimates based on mathematical modeling [32–36], while others have used prevalence in younger age groups or successive rounds of prevalence to estimate incidence [37–42]. Incidence estimates based on mathematical modeling are retrospective, not timely and have their biases. Additional limitations of modeling include inability to generate subgroup and risk factor analysis which are critical for understanding current transmission dynamics and for designing prevention strategies. In addition, increasing but variable ART coverage and decreasing mortality in most countries require input of additional but uncertain parameters into models, further contributing to potential biases.

In recent years, definitive progress has been made in the identification of new biomarkers and the development of assays, including molecular methods and rapid tests to detect and distinguish recent from long-term infections [5–7,43–46]. Reliable laboratory assays, if available, are attractive because of ease of use, application to cross-sectional population, low recruitment bias, low cost and provision of real-time incidence estimates. We recently described a novel, single-well limiting-antigen (LAg) avidity assay [5]. This novel concept was further developed into an optimized assay [6] and characterized with respect to its performance in multiple subtypes. Subsequently, we have transferred the assay to two commercial entities for development

of a kit and have conducted field evaluations in several populations worldwide in countries such as Vietnam, Ghana, Swaziland, and Kenya (to be published separately).

In March 2013, we organized a consultation meeting of experts to review data pertaining to characteristics, performance, and validation of the LAg-Avidity EIA. One of the recommendations included review of the mean duration of recent infection (MDRI) analysis. Although our previous report described the MDRI of 141 days at cutoff ODn of 1.0, our and others' subsequent work indicate that the method used to determine the MDRI was not applied optimally and recalibration of the assay was needed. We describe here the revised estimates of the MDRI using data from >250 seroconverters panels at various cut-offs using multiple statistical methods to ensure that these estimates are reliable and recommend a new MDRI at a preferred cut-off for application in cross-sectional incidence estimates.

## Materials and Methods

### Specimens

Longitudinal specimens (n = 2737) from 259 individuals infected with HIV-1 were collected as part of various cohort studies in different locales by different investigators. The specimens from consenting individuals were made available to permit development and characterization of new incidence assays, including the LAg-Avidity EIA. Some of the basic information about the cohorts, including source, number of seroconverters, available specimens, and likely or confirmed HIV-1 subtypes are shown in [Table 1](#). Of the 259 individuals, 89 of them (n = 393 specimens) were part of our previous study [6]. The following HIV-1 subtypes were included in this study: HIV-1 subtype B (Thailand BMA IDU cohort [47], Amsterdam cohort [48] and Trinidad cohort), subtype AE (Thailand BMA IDU cohort [47]), subtype C (Ethiopia and China cohorts), subtypes A & D (Kenya CSW cohort [49]). Because early antiretroviral therapy can affect the development and maturation of HIV antibodies, only specimens from persons who were not on antiretroviral therapy (ART) were used for determination of MDRI. Time between last negative and first positive specimens ranged from 4 days to 1486 days for different panels with median interval of 125 days and mean of 171 days.

An additional 3740 specimens from treatment-naïve adult individuals with HIV-1 infection longer than 1 year were used to estimate the proportion of specimens misclassified as recent, termed here as the proportion false recent (PFR). The specimens were collected under multiple approved protocols that permitted use of left-over, unlinked specimens for research. This set included 1845 specimens from Vietnam, 952 specimens from Ghana, 455 specimens from China and 488 specimens from individuals with AIDS (CD4<200). Specimens from individuals with AIDS were derived from three sources: 261 specimens were collected in the 1990s from treatment-naïve women with AIDS enrolled in the HIV Epidemiologic Research Study (HERS) [50], while additional specimens were from Thailand (n = 128) and Cote d'Ivoire (n = 99),

**Table 1. Country of origin, subtypes and specimens information for the seroconversion panels used in the study.**

Cohort	HIV-1 Subtypes	No. of Subjects	No. of Specimens
Netherlands, Trinidad, Thailand, US	B	69	704
Thailand	AE	97	1620
Ethiopia, China	C, BC, AE	59	332
Kenya	A, D	34	81
ALL	A, AE, B, C, BC and D	259	2737

doi:10.1371/journal.pone.0114947.t001

collected in the 1990s from treatment-naïve AIDS patients with (Cote d'Ivoire) or without (Thailand) tuberculosis (TB).

This study was conducted under a protocol approved by Centers for Disease Control and Prevention (CDC) Institutional Review Board (IRB) titled "characterization, validation and application of HIV-1 incidence assays". Selected specimens were collected under multiple CDC approved protocols (IRB # 5533, 5758). Study was also approved by Bangkok Metropolitan Administration Ethics Committee, respective ministries of health and CDC. Individuals donating the blood specimens provided written consent for use of the specimens for biological research.

## LAg-Avidity EIA

The LAg-Avidity EIA was performed as described earlier [6]. Following successful transfer of technology to a company, commercially produced kits were used to perform the testing (Sedia BioSciences, Portland, OR). These kits were verified as having the same performance characteristics as our in-house assay, including a matching Calibrator (CAL) specimen, a key to classification of recent and long-term infection. Details of the assay steps are as follows as per manufacturer's instructions: Assay controls [Negative control (NC), CAL, low-positive control (LPC) and high-positive control (HPC)] or HIV-positive specimens were diluted 1:101 in specimen diluent and 100  $\mu$ L of controls or specimens were added to appropriate wells of antigen-coated plates and incubated for 60 min at 37°C. Controls are included in duplicate (NC) or triplicate (other controls) on each plate, while specimens were tested in singlet. Plates were washed 4 times with 1x wash buffer to remove unbound antibodies. A pH 3.0 buffer was added to each well (200  $\mu$ L/well) and incubated for 15 min at 37°C to dissociate low avidity antibodies, if any. Following 4 washes, goat-anti-human IgG peroxidase (100  $\mu$ L/well) was added to each well and incubated for 30 min at 37°C. Tetramethyl benzidine substrate (100  $\mu$ L/well) was then added and incubated for 15 min at 25°C. Color development was stopped by addition of 100  $\mu$ L/well of 1N H<sub>2</sub>SO<sub>4</sub>. The optical density (OD) was read at 450 nm with 650 nm as a reference using a spectrophotometer.

Raw OD for each specimen was normalized using CAL OD on each plate as a ratio, such that normalized OD (OD<sub>n</sub>) = (OD of specimen/median OD of CAL). For the purpose of this exercise, all specimens were tested on two independent runs in singlet and the mean OD<sub>n</sub> was used for further analysis. Plates were validated using acceptable values of OD and OD<sub>n</sub> for each control and CAL as determined for the kit. If one or more of the controls fell outside of the acceptable ranges defined in the kit insert, the run was rejected. Specimens were then re-tested and OD<sub>n</sub> values from only valid runs were used for analysis. To assist with data management and analysis, an Excel-based data management tool was developed to auto-validate each plate, calculate OD<sub>n</sub> and classify specimens as recent or long-term infections based on 1.5 cutoff.

## Statistical Methods to Determine MDRI

Formally, the Mean Duration of Recent Infection (MDRI) of an assay, a required parameter of an assay to estimate incidence, is the mean time which subjects spend classified as 'recently infected' during a period T post-seroconversion. The Proportion of False Recent (PFR) result is a population-level probability of obtaining a 'recently infected' result on a randomly chosen person infected for more than time T which was set to one year [51]. We used seven different statistical approaches to derive the MDRI for the LAg assay at various cutoffs; they are presented below. Methods 1, 3, 6 and 7 assumed that the sero-conversion occurred at the mid-point of last negative and first positive dates while for methods 2, 4, and 5 sero-conversion was assumed

to have occurred at any time between the last negative and first positive dates with uniform probability.

Methods 1 and 2 (Empirical methods balancing false recent and false long-term): These two methods for estimating the mean duration of recent infection (MDRI) for the LAg Avidity assay use the “empirically balanced observation time” approach. The methods are based on some of the early work on incidence assays [3] suggesting that the rates for false-recents and false-long terms need to balance out, especially within the interval between 0 and 1 year ( $T = 365$  days) post-serconversion. Also for method 2, ODN values were raised to the power  $\lambda = 1.53$ , as estimated using a repeated measures model, in order to linearize the relationship between the ODN and time values. Daily values were determined by linear interpolation between time points or extrapolation from the last two points on either the untransformed (method 1) or on the transformed (method 2)  $ODN^\lambda$  scale. The baseline ODN value at day 0 was considered to be 0.05, equivalent to the background signal on the assay. Specimens from all serconversion panels, without exclusion, were used when applying these methods. Confidence intervals were determined by 10,000 replicate MDRI estimates obtained subject-level bootstrap resampling.

Method 3 (Linear interpolation [SACEMA-1]): This approach is based on linearly interpolating the LAg ODN values between visits, per subject. Each subject is assigned a reading of 0 at infection, and there is no extrapolation beyond the last visit. Using the interpolating readings,  $P_R(t)$ , which is the probability of testing ‘recent’ at time  $t$  post-infection, is estimated by the proportion of available results below the threshold at  $t$  post-infection.

Methods 4 & 5 (Binomial regression [SACEMA-2 and -3]): A linear binomial regression is used to model  $P_R(t)$ , as a function of time since infection,  $t$  [52]. Although the regression model does not account for the clustering of data points by subject, estimates of uncertainty through case bootstrap resampling do. The general form of the linear binomial regression model is  $g(p) = \beta^T x$ , where  $p$  is the probability of testing ‘recent’,  $g(\cdot)$  is the link function, and  $\eta = \beta^T x$  is the linear predictor ( $\beta$  is a vector of model parameters, and  $x$  is the vector of predictors). Two models were fitted: (i) A two-parameter model using a loglog link, where the linear predictor is a linear function of time (SACEMA-2); and (ii) a five-parameter model using a logit link, where  $x$  consists of the basis functions of a natural cubic spline over  $[0, T]$ , with knots occurring every two months (SACEMA-3). Data points more than  $T \times 110\%$  post-infection were not used in the fitting.

For both methods,  $\Omega_T = \int_0^T P_R(t) dt$  is then estimated using the composite trapezoidal rule for integration (20,000 subintervals). Assuming uniformly distributed infection times between last HIV-negative and first HIV-positive visits, the (expected) infection times are used (midpoints of inter-visit intervals), with no further accounting for uncertainty in infection times. Confidence interval (CI) limits are estimated by the percentiles of (1000) replicate MDRI estimates obtained by subject-level bootstrap resampling [53].

Method 6 (Nonparametric Survival Analysis): A nonparametric survival analysis method for interval-censored data was used to estimate the recency period of the assay. This approach required fewer assumptions than other approaches. It was adapted in our context where it was known that sero-conversion has occurred between two time points  $t_1$  and  $t_2$  and assay threshold was crossed between time points  $t_3$  and  $t_4$ , where  $t_1 \leq t_2 \leq t_3 \leq t_4$ . Therefore the recency period lies in the interval  $(t_3 - t_2)$  to  $(t_4 - t_1)$ . If the threshold was not crossed by the last observation then the upper end of this interval was set as censored. These two limits were used to calculate the maximum likelihood estimate of the survival curve. The mean estimates of the recency period were directly derived from the survival curve. For the mean to be defined finitely, it was assumed that the event occurred for the longest observed subject at the latest observed time. We employed a SAS macro called EMICM to estimate the survival curve for the recency



period [54]. Confidence intervals were estimated based on bootstrap techniques. Upper and lower limits of the interval were derived as 97.5<sup>th</sup> and 2.5<sup>th</sup> percentiles of the empirical distribution. Threshold values from 1.0 to 2.0 were used to derive MDR estimates for each of the subtypes and overall recency period.

Method 7 (Individual Panel Regression Analysis): Seroconversion (SC) panels were included in the analysis if they exhibited a rise in ODn response over the collection period and a regression equation could be fitted describing the antibody avidity kinetics. A total of 176 optimal SC panels comprising 2076 specimens were included in this analysis (Fig. 1B). Midpoint of last negative and first positive dates was used as the seroconversion date which was designated as day 0 and used to calculate days since seroconversion for subsequent longitudinal specimens. Each individual SC panel was plotted and a regression equation was generated using Excel. The regression equation was then solved for the desired cutoff value to determine estimated the number of days it required for that individual to reach the LAg assay cutoff. The mean duration of recent infection was then calculated by averaging the all SC panel results, along with the 95% CI for the mean. The mean duration of recent infection was calculated by subtype and overall, considering all subtypes. While the data requirements for this method are minimal, it does not use all the available data, such as the plateau data points which were not fully utilized.

## Determination of Proportion False Recent (PFR)

The PFR was determined as % of specimens collected more than one year post-seroconversion, which were misclassified as recent HIV-1 infection by the LAg-Avidity EIA. The PFR was calculated at each ODn cutoff of 1.0, 1.25, 1.5, 1.75 and 2.0 to evaluate the extent of misclassification at the various cutoffs. The 95% confidence intervals were calculated for each PFR.


## Results

### Antibody Avidity Kinetics

Antibody avidity maturation, as measured by LAg-Avidity EIA, for all 259 seroconverters is shown in Fig. 1A. Overall, there is an increase in avidity of gp41-specific antibodies following seroconversion, reaching a plateau level at about 500 days post-seroconversion. Most individuals exhibited normal increase in avidity kinetics; however, a few individuals showed some decline in antibody avidity over time while in rare cases antibody avidity remained low. Since statistical methods to calculate the MDRI can be affected by the duration between last negative and first positive results, collection interval, avidity kinetics and/or frequency of specimen collections, we separated optimal and sub-optimal seroconverter specimen sets. Fig. 1B shows 176 seroconverters (2076 specimens) with optimal time interval between last negative and first positive specimens (<100 days), with 3 or more specimens per donor with regular collection schedules, and also exhibiting a typical rise in antibody avidity levels. Fig. 1C shows 83 individuals (641 specimens) with one or more of the following when examined individually: sub-optimal collection schedules, longer time interval between last negative and first positive specimens (>100 days), or atypical antibody kinetics not crossing the potential cut-off threshold of ODn 1.0 to 2.0. It is interesting to note that when examined collectively, the antibody kinetics in Fig. 1C are not very different from those in Fig. 1B, except in rare cases when antibody avidity remained low, a likely contribution from elite controllers.

### MDRI and PFR Results

Analysis of the data by 7 different statistical methods for calculation of MDRI at varying cutoffs between ODn of 1.0 and 2.0 are summarized in Table 2. Overall, the different methods

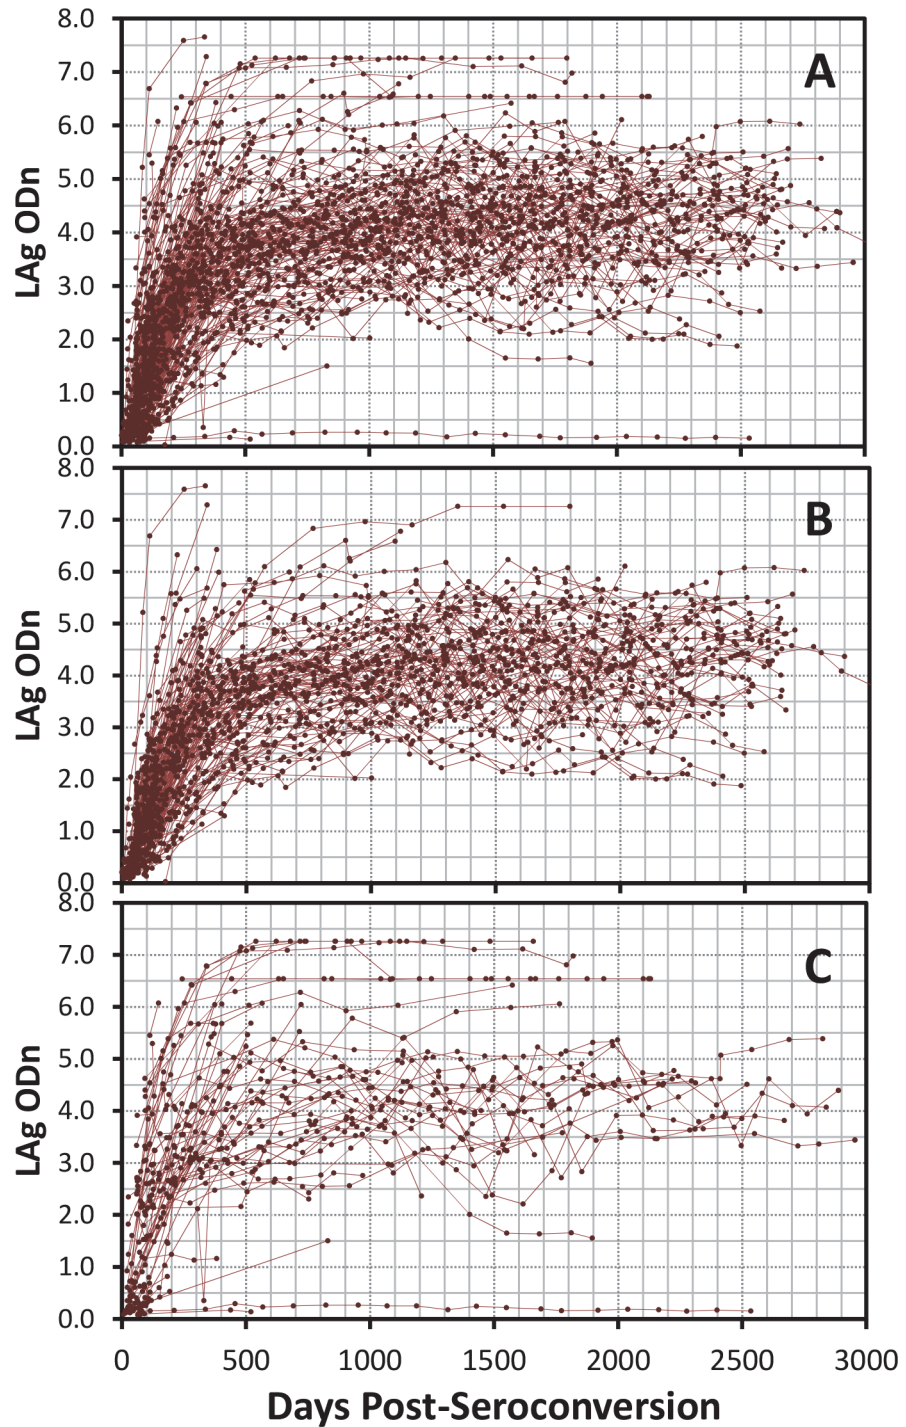

**Fig 1. A: Changes in antibody avidity as measured by LAG-Avidity EIA post-seroconversion for all 259 seroconversion panels.** For the purpose of these plots, midpoint of last negative and first positive dates for each panel was used as the seroconversion date to calculate days post-seroconversion (X-axis). B: Changes in avidity for 176 panels after exclusion of suboptimal panels as required by some methods. C: Changes in avidity as depicted for suboptimal panels that were excluded for some methods.

doi:10.1371/journal.pone.0114947.g001

**Table 2. Summary of 7 different methods used for determination of mean duration of recent infection (MDRI, in days with 95% CI) at varying cutoffs on LA<sub>g</sub>-Avidity EIA with corresponding level of proportion false recent (PFR) classification.**

MDRI Results of Different methods (1 to 7) Used								
Cutoff ODn	1	2	3	4	5	6	7	PFR (%)
1	91 (83–99)	87 (76–98)	92(79–104)	89 (81–98)	88 (78–98)	88 (79–98)	94(85–103)	0.6
1.25	114 (106–125)	110 (98–124)	113 (102–123)	110 (100–120)	110 (99–122)	109 (98–121)	112 (102–123)	1.0
1.5	137 (127–150)	133(121–149)	136 (122–150)	130 (119–141)	132 (120–144)	130 (118–142)	132 (121–143)	1.6
1.75	160 (150–174)	156.0 (143–173)	149 (135–164.0)	151(139–162)	147 (120–144)	145 (132–158)	155 (142–168)	1.9
2	183 (169–197)	177 (163–195)	171 (154–189)	171 (158–184)	166 (152–180)	161 (148–174)	181 (166–196)	2.5

See Methods section for further details of different methods used\*.

\*Methods 1 = Balanced time & 0,w and w,365, midpoint SC; 2 = Balanced time & 0,w and w,365, uniform SC; 3 = Non-Parametric MLE; 4 = Linear Interpolation; 5 = Binomial Regression (A); 6 = Binomial Regression (B); 7 = Individual SC Panel Regression. See Methods section for further details.

doi:10.1371/journal.pone.0114947.t002

provided similar results at each given cutoff. For example, at cutoff of 1.0 ODn, seven methods yield an MDRI of 87 to 94 days, while at cutoff of 1.5 ODn, the MDRI varied from 130 to 137 days. Corresponding misclassification (proportion false recent, PFR) among 3740 individuals with true long-term infections (>1 year) are shown in the right column (Table 2). This PFR represents overall misclassification frequency for all specimens, irrespective of subtypes or geographic locations. The PFR increased from 0.6% to 2.5% when threshold cutoff increased from 1.0 to 2.0 ODn, respectively. Subtype or country specific PFR data will be further analyzed in separate reports.

Differences of MDRI among different methods were minimal. Demonstratively, method 6, a binomial regression method that utilized all data points, indicated that at cutoff of 1.0 ODn, the MDRI was 88 days (95% CI 79–98) with a corresponding PFR of 0.6%, while at cutoff of 1.5 ODn, the MDRI was 130 days (95% CI 118–142) with a corresponding PFR of 1.6%. The MDRI increased to 161 days (95% CI 148–174) at cutoff of 2.0 ODn but there was a corresponding increase in PFR to 2.5%.


Fig. 2 shows MDRI by different subtypes or by geographic location (e.g., A&D from Kenya) using Method 6. MDRI by subtypes were: 129 days (subtype B), 122 days (subtype AE), 152 days (subtype C) and 109 days (subtypes A&D). Although there are some differences, use of an overall MDRI of 130 days (horizontal arrow) is appropriate for application to determine HIV-1 incidence in cross-sectional populations.

We examined the calculated MDRI (Method 6) at different cutoffs overlapping with the avidity kinetics during the early period of seroconversion (<500 days) as shown in Fig. 3. The line joining the MDRI at varying cutoff goes through the middle portion of the increasing avidity in this close up view of antibody maturation. The 95% CI around the MDRI are indicated with the red lines.

## Discussion

The MDRI is an essential characteristic of an incidence assay for appropriate application of the assay in cross-sectional estimation of the HIV-1 incidence. We previously reported optimization and characterization of LA<sub>g</sub>-Avidity EIA [6], including the determination of the MDRI using longitudinal specimens from 89 seroconverters. However, further review of the data indicated that the method used to calculate the MDRI was not properly applied to the dataset, resulting in an overestimate of the MDRI for the LA<sub>g</sub>-Avidity assay at the cutoff 1.0 ODn. Application of an elevated MDRI would result in an underestimation of HIV incidence if



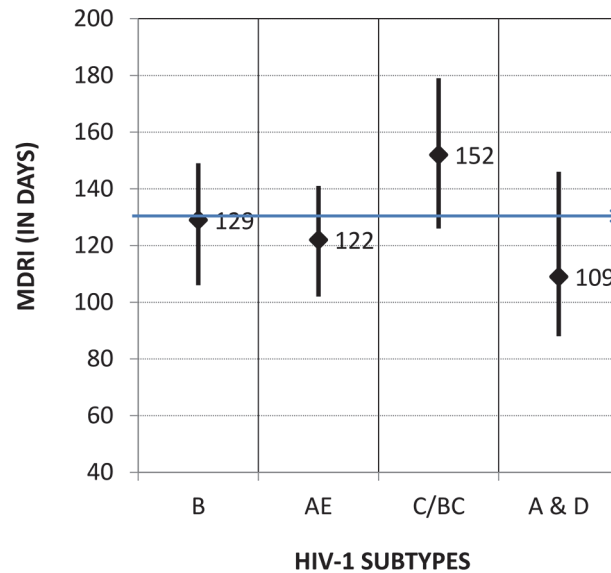


**Fig 2. Mean duration of recency at cutoff OD<sub>n</sub> of 1.5 by subtype or geographic region as determined by binomial regression method that uses all specimens without any exclusion criteria.** Closed diamonds represent MDRI for different subtypes and vertical lines represent upper and lower 95% CI. The horizontal line represents overall mean MDRI of 130 days.

doi:10.1371/journal.pone.0114947.g002

applied to a cross-sectional cohort. Therefore, this recalibration exercise was necessary and in order to achieve a more representative and robust estimate, we increased the number of seroconversion panels from 89 to >250 panels that represent more diverse subtypes and included multiple statistical methods to ensure accuracy and consensus of the final results.

In all, we used seven different statistical methods to determine the MDRI values and found that these methods gave very similar results providing further confidence to the robust nature of the analysis and the methods employed (Table 2). Our new results show that the MDRI of the LA<sub>g</sub>-Avidity EIA using the highlighted binomial regression method was 88 days and 161 days at the cutoffs of 1.0 to 2.0 OD<sub>n</sub>, respectively (Fig. 3). Determination of the optimal cutoff for cross-sectional application is a balance between MDRI (which should not be too small) and PFR (which should not be too large) [27,31,55,56]. At the cutoff of 1.5 OD<sub>n</sub>, our overall PFR was 1.6%, lower than 2% recommended by WHO Incidence Working Group [57] for new incidence assays. A cutoff of 1.5 OD<sub>n</sub> provides this balance between duration of MDRI (130 days) and PFR (<2.0%) using specimens in our collection. Therefore, we propose a default cutoff of 1.5 OD<sub>n</sub> to classify recent and long-term infections; this represents the mean duration of 130 days (95% CI 118–142) since seroconversion. It is recommended that the studies conducted previously with the LA<sub>g</sub>-Avidity EIA should reanalyze their data using revised cutoff (OD<sub>n</sub><1.5) for recent HIV infection classification and MDRI of 130 days as per our new analysis. This revision does not impact the raw data generated using the LA<sub>g</sub>-Avidity EIA, just the interpretation and use of the data.

Statistical methods used to determine MDRI have varied since the first description of the detuned assay in 1998 [9]. Since then multiple approaches have been used, partly due to lack of consensus among statisticians about the best methods [3,11,15,18,21,46,58]. Under the auspices of WHO Incidence Working Group, a statistical workshop was organized in 2011 to develop a consensus and promote a preferred method(s). Although there was some broad agreement and a better understanding of various approaches used, differences in the approaches remain, and no detailed benchmarking has been carried out. Recently, a benchmarking project has

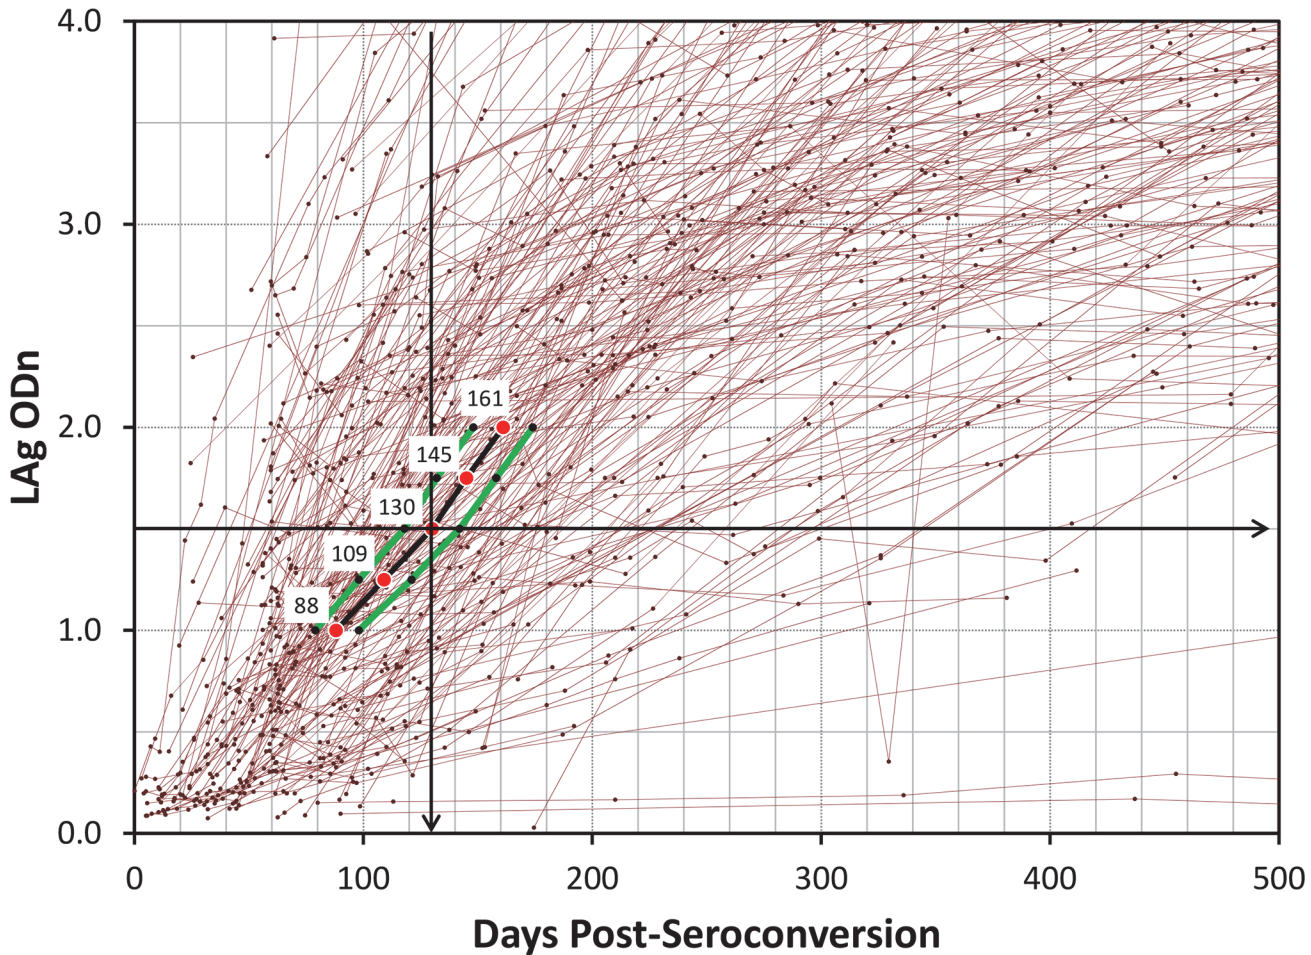

**Fig 3. Close-up view of changes in avidity with overlap of MDRI at cutoffs of 1.0 to 2.0 as determined by binomial regression method.** The red lines represent 95% bounds around MDRI.

doi:10.1371/journal.pone.0114947.g003

been launched under the auspices of the HIV Modeling Consortium (funded by the Bill and Melinda Gates Foundation) with a focus on identifying strengths and limitations of a diverse range of methods. Our analyses show that when used appropriately with a robust dataset, several of these methods yield comparable estimates of MDRI.

Comparison of the MDRI by HIV-1 subtypes/population show that the MDRI varied from 109 days (subtype A&D) to 152 days (subtype C). Further evaluation of the MDRI in more seroconversion panels collected from individuals infected with divergent HIV-1 subtypes and geographic locations should provide further data on subtype differences, if any. Such assessment by independent groups, such as CEPHIA, will be critical for this and other incidence assays. If subtype-specific differences are confirmed, use of MDRI for prevalent subtype is appropriate and may be considered when applying the LAG-Avidity EIA keeping in mind that trend of HIV incidence measured over time is more important than a single point estimate to assess the impact of HIV prevention efforts.

Although the PFR of 1.6% at the 1.5 ODn cutoff was below the recommended level of <2% in our study, this PFR was determined in ART-naïve populations. We realize that the actual PFR will vary in different populations depending on the state of the HIV epidemic, overall ART coverage, timing of ART initiation and duration of ART. Early initiation of treatment

before maturation of antibodies will prevent the development of high-avidity antibodies and will result in misclassification of long-term infections on most antibody-based assays, including LAg-Avidity EIA (unpublished data). Collection of additional clinical information about ART use during the surveys can help address this issue.

The continuing need to determine the local PFR during each round of survey is a burden for surveillance systems and can be impractical. False-recent classifications are caused primarily by elite controllers or individuals on treatment. Both of these cases can be effectively identified by testing for viral load, such that the LAg recent samples with VL < 1000 copies/mL, for example, would be classified as long-term. This approach is attractive for multiple reasons 1) it reduces the need to conduct exhaustive PFR studies, 2) it identifies misclassified elite controllers and those on ART in the study pool, and 3) it improves accuracy of incidence estimates. Given that this testing will be done only on LAg-recents (usually <10% of total positives) and many national reference laboratories in developing countries can now perform viral load testing, this is logistically feasible.

Recently, a multi-assay algorithm (MAA) has been suggested that includes 1) BED-capture EIA at a higher cutoff as the first step, followed by 2) Bio-Rad Avidity EIA, again at a higher cutoff 3) then CD4 measurement, and 4) finally VL measurement to classify recent HIV infection [52,59,60]. It is unclear how each of the multiple components of this somewhat complex algorithm contributes, whereas the relative simplicity of a single immunoassay and VL may suffice to provide sufficient precision. Additionally, any algorithm using CD4 will have limited application in surveys that collect dried blood spot (DBS) specimens for incidence testing. It should be pointed out that there are on-going developments in the area of HIV incidence algorithm development.

For wider application of the LAg-Avidity EIA to estimate HIV incidence, the next steps will include field validation of the revised parameters in cross-sectional populations and comparison of the LAg-derived estimates with other reference estimates of incidence in the same population. Further association of demographic and other risk factors in the context of HIV-1 incidence and prevalence should further assist in validation of the assay.

In summary, we have recalibrated the LAg-Avidity EIA using >250 longitudinal seroconversion panels from multiple subtypes derived from diverse geographical locations using several methods. Based on these data, we recommend a cutoff ODn of 1.5, which corresponds to an MDRI of 130 days (95% CI 118–142) for application in a cross-sectional population for estimation of HIV-1 incidence and risk-factor analysis. Determination of these parameters and recent availability of the assay kits from two manufacturers (Sedia BioSciences and Maxim BioMedical), including a dried blood spot (DBS) kit from the latter manufacturer, should further facilitate measurement of HIV-1 incidence in cross-sectional populations for program planning and impact evaluation of prevention and intervention efforts worldwide.

## Supporting Information

**S1 Table. Spreadsheet with LAg-Avidity EIA data on seroconversion panels (donors = 259; specimens = 2737) from multiple countries as described in Methods section.** Mean ODn of two independent runs was used for this analysis.  
(XLSX)

**S2 Table. Spreadsheet with LAg-Avidity EIA data on specimens from individuals (n = 3740) with known long-term infections (>1 year) for the purpose of determining proportion of false recent (PFR) classification.** Mean ODn of two independent runs was used for this analysis.  
(XLSX)

## Acknowledgments

This research has been supported by the President's Emergency Plan for AIDS Relief (PEPFAR) through the Centers for Disease Control and Prevention (CDC). The findings and conclusions in this report are those of the authors and do not necessarily represent the official position of the CDC/Agency for Toxic Substances and Disease Registry. AW and RK are grateful for support from the Bill and Melinda Gates Foundation through (and to their colleagues at) the Consortium for the Evaluation and Performance of HIV Incidence Assays, and the HIV Modeling Consortium.

## Author Contributions

Conceived and designed the experiments: BSP YD AAK NS YJ MQ. Performed the experiments: YD TD ER MQ HY YH. Analyzed the data: BSP YD RK AW M. Morgan AD YJ MQ NS. Contributed reagents/materials/analysis tools: BSP YD RK AW M. Morgan AD MEC CK BR M. Martin KC SV YJ MQ HY YH NS LL AAK TAN WA. Wrote the paper: BSP YD RK AW JN M. Morgan AD.

## References

1. Parekh BS, Hu DJ, Vanichseni S, Satten GA, Candal D, et al. (2001) Evaluation of a sensitive/less-sensitive testing algorithm using the 3A11-LS assay for detecting recent HIV seroconversion, among individuals with HIV-1 subtype B or E infection in Thailand. *AIDS Research & Human Retroviruses* 17: 453–458. doi: [10.1371/journal.pmed.1001777](https://doi.org/10.1371/journal.pmed.1001777) PMID: [25590520](https://pubmed.ncbi.nlm.nih.gov/25590520/)
2. Parekh BS, Pau CP, Kennedy MS, Dobbs TL, McDougal JS (2001) Assessment of antibody assays for identifying and distinguishing recent from long-term HIV type 1 infection. *AIDS Research & Human Retroviruses* 17: 137–146. doi: [10.1371/journal.pmed.1001777](https://doi.org/10.1371/journal.pmed.1001777) PMID: [25590520](https://pubmed.ncbi.nlm.nih.gov/25590520/)
3. Parekh BS, Kennedy MS, Dobbs T, Pau CP, Byers R, et al. (2002) Quantitative detection of increasing HIV type 1 antibodies after seroconversion: a simple assay for detecting recent HIV infection and estimating incidence. *AIDS Research & Human Retroviruses* 18: 295–307. doi: [10.1371/journal.pmed.1001777](https://doi.org/10.1371/journal.pmed.1001777) PMID: [25590520](https://pubmed.ncbi.nlm.nih.gov/25590520/)
4. Parekh BS, McDougal JS (2005) Application of laboratory methods for estimation of HIV-1 incidence. *Indian Journal of Medical Research* 121: 510–518. PMID: [15817960](https://pubmed.ncbi.nlm.nih.gov/15817960/)
5. Wei X, Liu X, Dobbs T, Kuehl D, Nkengasong JN, et al. (2010) Development of Two Avidity Based Assays to Detect Recent HIV-1 Seroconversion Using a Multi-subtype gp41 Recombinant Protein. *AIDS Research & Human Retroviruses* 26: 61–71. doi: [10.1371/journal.pmed.1001777](https://doi.org/10.1371/journal.pmed.1001777) PMID: [25590520](https://pubmed.ncbi.nlm.nih.gov/25590520/)
6. Duong YT, Qiu M, De AK, Jackson K, Dobbs T, et al. (2012) Detection of Recent HIV-1 Infection Using a New Limiting-Antigen Avidity Assay: Potential for HIV-1 Incidence Estimates and Avidity Maturation Studies. *PLoS One* 7: e33328. doi: [10.1371/journal.pone.0033328](https://doi.org/10.1371/journal.pone.0033328) PMID: [22479384](https://pubmed.ncbi.nlm.nih.gov/22479384/)
7. Granade TC, Nguyen S, Kuehl DS, Parekh BS (2013) Development of a novel rapid HIV test for simultaneous detection of recent or long-term HIV type 1 infection using a single testing device. *AIDS Res Hum Retroviruses* 29: 61–67. doi: [10.1089/aid.2012.0121](https://doi.org/10.1089/aid.2012.0121) PMID: [23281586](https://pubmed.ncbi.nlm.nih.gov/23281586/)
8. Soroka SD, Granade TC, Candal D, Parekh BS (2005) Modification of rapid human immunodeficiency virus (HIV) antibody assay protocols for detecting recent HIV seroconversion. *Clinical & Diagnostic Laboratory Immunology* 12: 918–921. doi: [10.1038/srep07632](https://doi.org/10.1038/srep07632) PMID: [25591183](https://pubmed.ncbi.nlm.nih.gov/25591183/)
9. Janssen RS, Satten GA, Stramer SL, Rawal BD, O'Brien TR, et al. (1998) New testing strategy to detect early HIV-1 infection for use in incidence estimates and for clinical and prevention purposes. [erratum appears in *JAMA* 1999 May 26;281(20):1893]. *JAMA* 280: 42–48. PMID: [9660362](https://pubmed.ncbi.nlm.nih.gov/9660362/)
10. Kothe D, Byers RH, Caudill SP, Satten GA, Janssen RS, et al. (2003) Performance characteristics of a new less sensitive HIV-1 enzyme immunoassay for use in estimating HIV seroincidence. *Journal of Acquired Immune Deficiency Syndromes: JAIDS* 33: 625–634. PMID: [12902808](https://pubmed.ncbi.nlm.nih.gov/12902808/)
11. Barin F, Meyer L, Lancar R, Deveau C, Gharib M, et al. (2005) Development and validation of an immunoassay for identification of recent human immunodeficiency virus type 1 infections and its use on dried serum spots. *Journal of Clinical Microbiology* 43: 4441–4447. PMID: [16145089](https://pubmed.ncbi.nlm.nih.gov/16145089/)
12. Suligoi B, Galli C, Massi M, Di Sora F, Sciandra M, et al. (2002) Precision and accuracy of a procedure for detecting recent human immunodeficiency virus infections by calculating the antibody avidity index by an automated immunoassay-based method. *Journal of Clinical Microbiology* 40: 4015–4020. PMID: [12409368](https://pubmed.ncbi.nlm.nih.gov/12409368/)



13. Suligoi B, Massi M, Galli C, Sciandra M, Di Sora F, et al. (2003) Identifying recent HIV infections using the avidity index and an automated enzyme immunoassay. *Journal of Acquired Immune Deficiency Syndromes: JAIDS* 32: 424–428. PMID: [12640201](#)
14. Suligoi B, Rodella A, Raimondo M, Regine V, Terlenghi L, et al. (2011) Avidity Index for anti-HIV antibodies: comparison between third- and fourth-generation automated immunoassays. *J Clin Microbiol* 49: 2610–2613. doi: [10.1128/JCM.02115-10](#) PMID: [21543577](#)
15. Wilson KM, Johnson EI, Croom HA, Richards KM, Doughty L, et al. (2004) Incidence immunoassay for distinguishing recent from established HIV-1 infection in therapy-naive populations. *AIDS* 18: 2253–2259. PMID: [15577537](#)
16. Constantine NT, Sill AM, Jack N, Kreisel K, Edwards J, et al. (2003) Improved classification of recent HIV-1 infection by employing a two-stage sensitive/less-sensitive test strategy. *Journal of Acquired Immune Deficiency Syndromes: JAIDS* 32: 94–103. PMID: [12514420](#)
17. Li H, Ketema F, Sill AM, Kreisel KM, Cleghorn FR, et al. (2007) A simple and inexpensive particle agglutination test to distinguish recent from established HIV-1 infection. *International Journal of Infectious Diseases* 11: 459–465. PMID: [17369067](#)
18. Sill AM, Kreisel K, Deeds BG, Wilson CM, Constantine NT, et al. (2007) Calibration and validation of an oral fluid-based sensitive/less-sensitive assay to distinguish recent from established HIV-1 infections. *Journal of Clinical Laboratory Analysis* 21: 40–45. PMID: [17245763](#)
19. Hargrove JW, Humphrey JH, Mutasa K, Parekh BS, McDougal JS, et al. (2008) Improved HIV-1 incidence estimates using the BED capture enzyme immunoassay. *AIDS* 22: 511–518. doi: [10.1097/QAD.0b013e3282f2a960](#) PMID: [18301064](#)
20. Kim AA, McDougal JS, Hargrove J, Rehle T, Pillay-Van Wyk V, et al. (2010) Evaluating the BED capture enzyme immunoassay to estimate HIV incidence among adults in three countries in sub-Saharan Africa. *AIDS Res Hum Retroviruses* 26: 1051–1061. doi: [10.1089/aid.2009.0218](#) PMID: [20849299](#)
21. Parekh BS, Hanson DL, Hargrove J, Branson B, Green T, et al. (2011) Determination of mean recency period for estimation of HIV type 1 Incidence with the BED-capture EIA in persons infected with diverse subtypes. *AIDS Res Hum Retroviruses* 27: 265–273. doi: [10.1089/aid.2010.0159](#) PMID: [20954834](#)
22. Guy R, Gold J, Calleja JMG, Kim AA, Parekh B, et al. (2009) Accuracy of serological assays for detection of recent infection with HIV and estimation of population incidence: a systematic review. *The Lancet Infectious Diseases* 9: 747–759. doi: [10.1016/S1473-3099\(09\)70300-7](#) PMID: [19926035](#)
23. Young CL, Hu DJ, Byers R, Vanichseni S, Young NL, et al. (2003) Evaluation of a sensitive/less sensitive testing algorithm using the bioMerieux Vironostika-LS assay for detecting recent HIV-1 subtype B' or E infection in Thailand. *AIDS Research & Human Retroviruses* 19: 481–486. doi: [10.1371/journal.pmed.1001777](#) PMID: [25590520](#)
24. Barnighausen T, McWalter TA, Rosner Z, Newell ML, Welte A (2010) HIV incidence estimation using the BED capture enzyme immunoassay: systematic review and sensitivity analysis. *Epidemiology* 21: 685–697. doi: [10.1097/EDE.0b013e3181e9e978](#) PMID: [20699682](#)
25. Hallett TB, Ghys P, Barnighausen T, Yan P, Garnett GP (2009) Errors in 'BED'-derived estimates of HIV incidence will vary by place, time and age. *PLoS ONE [Electronic Resource]* 4: e5720. doi: [10.1371/journal.pone.0005720](#) PMID: [19479050](#)
26. McDougal JS, Pilcher CD, Parekh BS, Gershny-Damet G, Branson BM, et al. (2005) Surveillance for HIV-1 incidence using tests for recent infection in resource-constrained countries. *AIDS* 19 Suppl 2: S25–30. PMID: [15930838](#)
27. Busch MP, Pilcher CD, Mastro TD, Kaldor J, Vercauteren G, et al. (2010) Beyond detuning: 10 years of progress and new challenges in the development and application of assays for HIV incidence estimation. *AIDS* 24: 2763–2771. doi: [10.1097/QAD.0b013e32833f1142](#) PMID: [20975514](#)
28. Mastro TD, Kim AA, Hallett T, Rehle T, Welte A, et al. (2010) Estimating HIV Incidence in Populations Using Tests for Recent Infection: Issues, Challenges and the Way Forward. *J HIV AIDS Surveill Epidemiol* 2: 1–14. PMID: [21743821](#)
29. Mastro TD (2013) Determining HIV incidence in populations: moving in the right direction. *J Infect Dis* 207: 204–206. doi: [10.1093/infdis/jis661](#) PMID: [23129757](#)
30. Smolen-Dzirba J, Wasik TJ (2011) Current and future assays for identifying recent HIV infections at the population level. *Med Sci Monit* 17: RA124–133. PMID: [21525823](#)
31. Welte A, McWalter TA, Laeyendecker O, Hallett TB (2010) Using tests for recent infection to estimate incidence: problems and prospects for HIV. *Euro Surveill* 15.
32. Hladik W, Musinguzi J, Kirungi W, Opio A, Stover J, et al. (2008) The estimated burden of HIV/AIDS in Uganda, 2005–2010. *AIDS* 22: 503–510. doi: [10.1097/QAD.0b013e3282f470be](#) PMID: [18301063](#)



33. Kim AA, Hallett T, Stover J, Gouws E, Musinguzi J, et al. (2011) Estimating HIV incidence among adults in Kenya and Uganda: a systematic comparison of multiple methods. *PLoS ONE* 6: e17535. doi: [10.1371/journal.pone.0017535](https://doi.org/10.1371/journal.pone.0017535) PMID: [21408182](https://pubmed.ncbi.nlm.nih.gov/21408182/)
34. Heimer R (2008) Community coverage and HIV prevention: assessing metrics for estimating HIV incidence through syringe exchange. *International Journal of Drug Policy* 19 Suppl 1: S65–73. doi: [10.1016/j.drugpo.2007.12.004](https://doi.org/10.1016/j.drugpo.2007.12.004) PMID: [18207726](https://pubmed.ncbi.nlm.nih.gov/18207726/)
35. Brown T, Bao L, Raftery AE, Salomon JA, Baggaley RF, et al. (2010) Modelling HIV epidemics in the antiretroviral era: the UNAIDS Estimation and Projection package 2009. *Sex Transm Infect* 86 Suppl 2: ii3–10. doi: [10.1136/sti.2010.044784](https://doi.org/10.1136/sti.2010.044784) PMID: [20929855](https://pubmed.ncbi.nlm.nih.gov/20929855/)
36. UNAIDS (2010) UNAIDS Report on the global AIDS epidemic 2010. Joint United Nations Programme on HIV/AIDS (UNAIDS).
37. Hallett TB, Zaba B, Todd J, Lopman B, Mwita W, et al. (2008) Estimating incidence from prevalence in generalised HIV epidemics: methods and validation. *PLoS Medicine / Public Library of Science* 5: e80.
38. Hallett TB, Singh K, Smith JA, White RG, Abu-Raddad LJ, et al. (2008) Understanding the impact of male circumcision interventions on the spread of HIV in southern Africa. *PLoS ONE [Electronic Resource]* 3: e2212. doi: [10.1371/journal.pone.0002212](https://doi.org/10.1371/journal.pone.0002212) PMID: [18493593](https://pubmed.ncbi.nlm.nih.gov/18493593/)
39. Hoare A, Wilson DP, Regan DG, Kaldor J, Law MG (2008) Using mathematical modelling to help explain the differential increase in HIV incidence in New South Wales, Victoria and Queensland: importance of other sexually transmissible infections. *Sexual Health* 5: 169–187. PMID: [18686336](https://pubmed.ncbi.nlm.nih.gov/18686336/)
40. Walker PT, Hallett TB, White PJ, Garnett GP (2008) Interpreting declines in HIV prevalence: impact of spatial aggregation and migration on expected declines in prevalence. *Sexually Transmitted Infections* 84 Suppl 2: ii42–48. doi: [10.1136/sti.2008.029975](https://doi.org/10.1136/sti.2008.029975) PMID: [18799492](https://pubmed.ncbi.nlm.nih.gov/18799492/)
41. Wilson DP, Hoare A, Regan DG, Law MG (2009) Importance of promoting HIV testing for preventing secondary transmissions: modelling the Australian HIV epidemic among men who have sex with men. *Sexual Health* 6: 19–33. PMID: [19254488](https://pubmed.ncbi.nlm.nih.gov/19254488/)
42. Chemaitelly H, Abu-Raddad LJ (2013) External infections contribute minimally to HIV incidence among HIV sero-discordant couples in sub-Saharan Africa. *Sex Transm Infect* 89: 138–141. doi: [10.1136/sextrans-2012-050651](https://doi.org/10.1136/sextrans-2012-050651) PMID: [22930346](https://pubmed.ncbi.nlm.nih.gov/22930346/)
43. Andersson E, Shao W, Bontell I, Cham F, Cuong DD, et al. (2013) Evaluation of sequence ambiguities of the HIV-1 pol gene as a method to identify recent HIV-1 infection in transmitted drug resistance surveys. *Infect Genet Evol* 18C: 125–131.
44. Curtis KA, Kennedy MS, Charurat M, Nasidi A, Delaney K, et al. (2012) Development and Characterization of a Bead-Based, Multiplex Assay for Estimation of Recent HIV Type 1 Infection. *AIDS Res Hum Retroviruses* 28: 188–197. doi: [10.1089/AID.2011.0037](https://doi.org/10.1089/AID.2011.0037) PMID: [21585287](https://pubmed.ncbi.nlm.nih.gov/21585287/)
45. Sharma UK, Schito M, Welte A, Rousseau C, Fitzgibbon J, et al. (2012) Workshop Summary: Novel Biomarkers for HIV Incidence Assay Development. *AIDS Res Hum Retroviruses*.
46. Ragonnet-Cronin M, Aris-Brosou S, Joannis I, Merks H, Vallee D, et al. (2012) Genetic diversity as a marker for timing infection in HIV-infected patients: evaluation of a 6-month window and comparison with BED. *J Infect Dis* 206: 756–764. doi: [10.1093/infdis/jis411](https://doi.org/10.1093/infdis/jis411) PMID: [22826337](https://pubmed.ncbi.nlm.nih.gov/22826337/)
47. Hudgens MG, Longini IM Jr, Vanichseni S, Hu DJ, Kitayaporn D, et al. (2002) Subtype-specific transmission probabilities for human immunodeficiency virus type 1 among injecting drug users in Bangkok, Thailand. *American Journal of Epidemiology* 155: 159–168. PMID: [11790680](https://pubmed.ncbi.nlm.nih.gov/11790680/)
48. van Griensven G, Tielman RA, Goudsmit J, van der Noordaa J, de Wolf F, et al. (1987) Risk factors and prevalence of HIV antibodies in homosexual men in the Netherlands. *American J of Epidemiology* 125: 1048–1057. PMID: [3495173](https://pubmed.ncbi.nlm.nih.gov/3495173/)
49. Ludo L, Baeten JM, Kreiss JK, Richardson BA, Chohan BH, et al. (2004) Injectable contraceptive use and genital ulcer disease during the early phase of HIV-1 infection increase plasma virus load in women. *Journal of Infectious Diseases* 189: 303–311. PMID: [14722896](https://pubmed.ncbi.nlm.nih.gov/14722896/)
50. Smith D, Warren DL, Vlahov D, Schuman P, Stein MD, et al. for the Human Immunodeficiency Virus Epidemiology Research Study Group (1997) Design and baseline participant characteristics of the Human Immunodeficiency Virus Epidemiology Research (HER) Study: a prospective cohort study of human immunodeficiency virus infection in US women. *Am J epidemiology* 146: 459–469. PMID: [9290506](https://pubmed.ncbi.nlm.nih.gov/9290506/)
51. Kassanjee R, McWalter TA, Barnighausen T, Welte A (2012) A new general biomarker-based incidence estimator. *Epidemiology* 23: 721–728. doi: [10.1097/EDE.0b013e3182576c07](https://doi.org/10.1097/EDE.0b013e3182576c07) PMID: [22627902](https://pubmed.ncbi.nlm.nih.gov/22627902/)
52. Brookmeyer R, Konikoff J, Laeyendecker O, Eshleman SH (2013) Estimation of HIV incidence using multiple biomarkers. *Am J Epidemiol* 177: 264–272. doi: [10.1093/aje/kws436](https://doi.org/10.1093/aje/kws436) PMID: [23302151](https://pubmed.ncbi.nlm.nih.gov/23302151/)
53. Efron B, Tibshirani RJ (1993) *An Introduction to the Bootstrap*: Chapman & Hall/CRC.

54. Ying S, Gordon J, Se HK. Analyzing Interval-Censored Survival Data with SAS Software. In: Inc. SI, editor; 2010; Cary, NC.
55. Hallett TB (2011) Estimating the HIV incidence rate: recent and future developments. *Curr Opin HIV AIDS* 6: 102–107. doi: [10.1097/COH.0b013e328343bdfb](https://doi.org/10.1097/COH.0b013e328343bdfb) PMID: [21505383](https://pubmed.ncbi.nlm.nih.gov/21505383/)
56. Incidence Assay Critical Path Group (2011) More and better information to tackle HIV epidemics: towards improved HIV incidence assays. *PLoS Medicine / Public Library of Science* 8(6):e1001045. doi: [10.1371/journal.pmed.1001045](https://doi.org/10.1371/journal.pmed.1001045) PMID: [21731474](https://pubmed.ncbi.nlm.nih.gov/21731474/)
57. WHO/UNAIDS (2012) UNAIDS/WHO Working Group on Global HIV/AIDS and STI Surveillance. When and how to use assays for recent infection to estimate HIV incidence at a population level.
58. Sweeting M, Angelis DD, Parry P, and Suligoi B (2010) Estimating the distribution of the window period for recent HIV infections: a comparison of statistical methods. *Statistics in Medicine* DOI: 10.1002/sim.0000.
59. Laeyendecker O, Brookmeyer R, Cousins MM, Mullis CE, Konikoff J, et al. (2013) HIV incidence determination in the United States: a multiassay approach. *J Infect Dis* 207: 232–239. doi: [10.1093/infdis/jis659](https://doi.org/10.1093/infdis/jis659) PMID: [23129760](https://pubmed.ncbi.nlm.nih.gov/23129760/)
60. Eshleman SH, Hughes JP, Laeyendecker O, Wang J, Brookmeyer R, et al. (2013) Use of a multifaceted approach to analyze HIV incidence in a cohort study of women in the United States: HIV Prevention Trials Network 064 Study. *J Infect Dis* 207: 223–231. doi: [10.1093/infdis/jis658](https://doi.org/10.1093/infdis/jis658) PMID: [23129758](https://pubmed.ncbi.nlm.nih.gov/23129758/)

Copyright of PLoS ONE is the property of Public Library of Science and its content may not be copied or emailed to multiple sites or posted to a listserv without the copyright holder's express written permission. However, users may print, download, or email articles for individual use.