


RESEARCH ARTICLE

Acceptability, feasibility, and accuracy of blood-based HIV self-testing: A cross-sectional study in Ho Chi Minh City, Vietnam

Bao Vu Ngoc^{1*}, Mohammed Majam², Kimberly Green¹, Ton Tran³, Minh Tran Hung⁴, Anh Luong Que³, Diep Bui Ngoc⁴, Chuong Hoang Le Duy³

1 PATH, Hanoi, Vietnam, **2** Ezintsha, Wits Health Consortium, University of the Witwatersrand, Johannesburg, South Africa, **3** Pasteur Institute, Ho Chi Minh City, Vietnam, **4** Center for Creative Initiatives in Health and Population, Hanoi, Vietnam

* [bvuv@path.org](mailto:bvu@path.org)



Abstract

HIV self-testing (HIVST) is an effective approach to increase testing uptake. While oral fluid-based HIVST has been rapidly scaled, use of blood-based HIVST remains limited. We evaluated the acceptability, feasibility, and accuracy of blood-based HIVST among lay users in Ho Chi Minh City (HCMC), Vietnam. We conducted a cross-sectional study among HIV testing clients at the HCMC Pasteur Institute from March 2019 to October 2020. Participants received one HIVST kit and performed the test in front of an observer. The observer used product-specific questionnaires to collect information on the HIVST process, test results, experiences. The participants' interpretations of HIVST results were compared to health staff's interpretations and gold standard laboratory EIA reference tests. Of 2,399 participants who accepted HIVST, 64.7% were men, 62.1% aged 25–49 years, 53.5% had a higher education level, 41.4% were employed, and 35.6% were first-time testers. The vast majority (94.4%) desired to use the test in the future, and 93.9% reported willingness to recommend the test. The majority (90.8%) of participants successfully completed the self-test. One factor associated with successful completion was higher education level (aOR = 1.85; 95% CI: 1.32–2.61); while participants self-testing with SURE CHECK (aOR = 0.21; 95% CI: 0.12–0.37), INSTI (aOR = 0.23; 95% CI: 0.13–0.39), and BioSURE (aOR = 0.29; 95% CI: 0.17–0.51) or being unemployed, retired, or doing housework (aOR = 0.45; 95% CI: 0.25–0.82) were less likely to perform the test successfully. Agreement of positive and negative HIVST results as interpreted by participants and health staff was high (98.1% and 99.9%, respectively). Sensitivity and specificity of the evaluated HIVST were 96.43% (95% CI: 93.62–99.23) and 99.9% (95% CI: 99.75–100), respectively. Our findings confirm that blood-based HIVST is highly acceptable, feasible, and accurate. This evidence informs scale-up of HIVST to increase uptake of essential HIV prevention and treatment services.

OPEN ACCESS

Citation: Ngoc BV, Majam M, Green K, Tran T, Hung MT, Que AL, et al. (2023) Acceptability, feasibility, and accuracy of blood-based HIV self-testing: A cross-sectional study in Ho Chi Minh City, Vietnam. *PLOS Glob Public Health* 3(2): e0001438. <https://doi.org/10.1371/journal.pgph.0001438>

Editor: Elisa Lopez-Varela, Barcelona Institute for Global Health: Instituto de Salud Global Barcelona, SPAIN

Received: September 15, 2022

Accepted: December 28, 2022

Published: February 1, 2023

Copyright: © 2023 Ngoc et al. This is an open access article distributed under the terms of the [Creative Commons Attribution License](https://creativecommons.org/licenses/by/4.0/), which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.

Data Availability Statement: All relevant data are within the manuscript and its [Supporting Information](#) files. DOI: [10.6084/m9.figshare.21755810](https://doi.org/10.6084/m9.figshare.21755810).

Funding: This work was supported by the Bill & Melinda Gates Foundation (OPP1132929 to MM; subagreement between Wits Reproductive Health and HIV Institute - A division of Wits Health Consortium (Pty) Ltd and PATH to BVN, KG, TT,

MTH, ALQ, DBN, CHLD). The funders had no role in the study design, data collection and analysis, decision to publish, or preparation of the manuscript.

Competing interests: The authors have declared that no competing interests exist.

Introduction

HIV self-testing (HIVST) has been emerging as an effective approach to access unreached populations for HIV testing services [1]. HIVST is a self-care intervention grounded in a person-centered approach as part of primary health care that improves the coverage of testing and supports a continuum of care for persons at risk for or living with HIV [2]. HIVST is also essential for maintaining delivery of essential services, such as HIV testing and access to treatment and pre-exposure prophylaxis (PrEP), particularly during times of COVID-19 social distancing [1,3].

Multi-country evidence confirms the high acceptability, feasibility, and accuracy of HIVST across populations with minimal harm [1,4–13]. HIVST is highly acceptable due to its convenience, privacy, confidentiality, and ease of use [14–16]. Although studies report oral fluid-based HIVST was preferred because of its ease of use and it being noninvasive and painless [17–23], little is known about blood-based HIVST. The most common errors by lay users of blood-based HIVST include failing to prepare the test kit correctly, taking the blood sample incorrectly, and spilling the buffer solution [17,24–26]. Factors associated with the ability to successfully perform or interpret an HIVST result include higher education level, younger age, prior experience with HIV testing, and training prior to taking the test, as well as the location of the study site being in an upper-income neighborhood [6,27,28]. Concordance between blood-based self-test results as read by lay users versus as read by health care workers is high [25,29–32]. In a usability study of seven HIVST devices, including five finger-stick blood-based kits (Atomo generation 1 and generation 2, INSTI, BioSURE, and SURE CHECK), Majam et al. found that the average usability index was 92.8% (84.2%–97.6%), and the main difficulty reported by participants was in obtaining and transferring specimens; participants correctly interpreted 96.1% of the nonreactive results, 97.0% of the reactive results, 98.0% of the invalid results, and 79.9% of the weak positive results [31].

The sensitivity and specificity of HIVST kits vary by kit type. A systematic review and meta-analysis found that sensitivity and specificity were higher for blood-based HIVST compared with oral fluid-based HIVST [10,11,13]. A performance study of OraQuick HIVST compared to a fourth-generation laboratory reference in Zambia reported sensitivity of 87.5% and specificity of 99.7% [13]. In a recent performance assessment of four HIVST devices, including three blood-based HIVST kits (BioSURE, INSTI, and SURE CHECK), and one oral HIVST kit (OraQuick), Majam et al. reported the sensitivity and specificity were 99.7% and 100%, 99% and 100%, 96.8% and 100%, and 99.3% and 99.4%, respectively [33].

In terms of willingness to pay (WTP) for HIVST, there is mismatch between the price and the WTP for HIVST in low- and middle-income countries (LMICs). The price per HIVST kit ranged from US\$2–\$12 in the public sector and from US\$7–\$12 in the private sector [34], while most people were willing to pay less than US\$7 (e.g., US\$0.1–\$6.3 in South Africa, US\$1–\$1.25 in Kenya, US\$1.77 in Cote d'Ivoire, US\$0.84 in Tanzania, and US\$3 in Cambodia) [10,18,35–37]. WTP varied across key populations and countries. For example, men who have sex with men (MSM) were willing to pay US\$10 in the Philippines, US\$6.5 in China, or US\$5.5 in Nigeria, while female sex workers (FSW) were willing to pay US\$4.8 in China or US\$0.3–\$2.88 in Uganda [38–42]. Our previous study in Vietnam also found that MSM were willing to pay more than FSW and people who inject drugs (PWID) (US\$4.6, US\$3.2, and US\$2.3, respectively) [43].

Many barriers prevent the adoption and scale-up of HIVST in LMICs, including concerns over accuracy, feasibility, acceptability, and cost of HIVST [15,25,26,44]. WHO recommended that all HIV testing algorithms achieve at least 99% positive predictive value and use a combination of tests with at least 99% sensitivity and 98% specificity to maintain the accuracy and

reliability of HIV diagnosis [1]. While HIV rapid diagnostic tests (RDTs) are historically performed by trained health care workers and thus yield high sensitivity and specificity, RDTs packaged for self-testing and performed by lay users may lead to different accuracies in test results. As such, the WHO requirements for sensitivity and specificity limit registration and scale-up of HIVST products in LMICs. Moreover, blood-based HIVST is not as widely available and may not be as accepted as oral fluid-based HIVST, while the current price of most blood-based HIVST kits exceeds what people in LMICs are WTP. COVID-19 has only exacerbated challenges with access to HIV testing. The Global Fund reported a 22% drop in HIV testing from 2019 to 2020 across ten countries that report the largest volume of testing. In some settings, HIVST access has been increased successfully to address these gaps [45,46].

Our research questions include: (1) Do users accept blood-based HIVST, what are their preferences, and what is their WTP for blood-based HIVST; (2) can lay users perform blood-based HIVST correctly; and (3) what is the sensitivity and specificity of blood-based HIVST kits when performed by lay users?

In this paper, we present findings from the usability and performance assessment of four blood-based HIVST kits in Vietnam, with a focus on the acceptability, feasibility, and accuracy of HIVST in the hands of lay users. The assessment was funded by the Bill & Melinda Gates Foundation and implemented by PATH in collaboration with Ezintsha, Wits Health Consortium, University of Witwatersrand, Johannesburg, South Africa, and the Pasteur Institute in Ho Chi Minh City, Vietnam.

Materials and methods

Ethics statement

Ethical approval was obtained from the PATH Research Ethics Committee (reference number 1326168–2 and 1542399–2) and the Ho Chi Minh City Pasteur Institute Research Ethics Committee (reference number 78/GCN-PAS and 17/GCN-PAS). Written informed consent was obtained from study participants. All participants provided written informed consent and there were no refusals.

Study design

We conducted a cross-sectional study to assess the usability and performance of blood-based HIVST. The primary outcomes of interest were the usability, acceptability, feasibility, and accuracy of blood-based HIVST kits in the hands of unassisted lay users. **Usability** was defined as the number and percentage of participants who completed all testing steps correctly without assistance and interpreted the results correctly. **Acceptability** was measured through acceptance of HIVST, willingness to recommend the test, desire to use the test in the future, preference for use of the test, and WTP for HIVST. **Feasibility** was measured by the ability of lay users to correctly use the self-test, succeed in obtaining an interpretable result, and correctly interpret the results. **Accuracy** was estimated by the sensitivity and specificity of HIVST kits compared to the gold standard enzyme immunoassay (EIA) or enzyme-linked immunosorbent assay (ELISA) test (i.e., Murex HIV Ag/Ab Combination).

As no standardized questionnaires for investigating the usability of HIVST for prequalification were available at the time of the study, we developed the product-specific semi-structured questionnaire (S1, S2, S3, and S4 Text) based on WHO prequalification literature [47]. The questionnaire was piloted in a sample of 50 participants for each HIVST device. Findings of the pilot were shared with the manufacturers for their feedback to incorporate in the final questionnaires. None of the manufacturers chose to amend their instructions for use of the product before the study was commenced.

HIV self-test kits

Four blood-based HIVST devices were assessed: INSTI (bioLytical Laboratories, Canada), SURE CHECK (Chembio Diagnostic Systems, USA), BioSURE (BioSure Ltd., United Kingdom), and CheckNOW (Abbott Diagnostics, USA). Each HIVST device included the manufacturer's instructions-for-use (IFU) and other kit components. No additional job aids, demonstrations, or assistance were provided.

Study population

Our study population was made up of clients seeking fee-based HIV testing services at the HCMC Pasteur Institute that included either general population or key populations who didn't want to seek free HIV testing services currently offered by community-based organizations or district health centers under the U.S. President's Emergency Plan for AIDS Relief and the Global Fund to Fight AIDS, Tuberculosis, and Malaria-supported projects in the city. Study participants were required to be age 18 years or older, first-time HIV self-testers with a self-reported unknown or HIV-negative status, and proficient in speaking and reading Vietnamese. Clients were excluded if they had any prior experience with HIVST, were health care workers or lay providers who provided HIV testing services, were currently on PrEP or antiretroviral medication treatment, had a known HIV-positive status, and/or had any extenuating conditions (e.g., acute illness) that would interfere with the study process.

Sample size and sampling

A sample size of up to 600 participants per product was required for the usability and sensitivity assessment of each device, as per WHO technical guidance [48]. All clients who came to the Institute for an HIV test during the study period were invited to participate in this study. The "take all" method was applied to recruit study participants. The recruitment was consecutively carried out until it reached the expected sample size for each type of HIV test. Total sample size estimated was 2,400 study participants, 600 for each HIVST device.

Data collection

The data collection was conducted by a research team consisting of eight health staff (lab technicians and nurses) from March 2019 to October 2020. Clients visiting the examination department went through a routine registration procedure. If a client opted for HIVST, they were provided with a written recruitment script. The research nurse verbally obtained their consent for participation in a study enrollment screening process that retrieved information such as age, education, employment status, dominant hand, visual status, and historical and current use of HIV testing and antiretroviral drugs. They registered the client in a biometric enrollment system. Clients agreeing to the screening process were screened for eligibility based on the inclusion and exclusion criteria. The nurse explained the research and covered all the required elements of consent. Eligible participants were also given an informed consent form to read. Participants were encouraged to ask questions to ensure the entire process was clearly understood. If clients agreed to participate in the study, they were asked to sign the consent form. Eligible participants also provided a fingerprint scan to eliminate duplication of enrolled participants.

Study participants were handed one HIVST kit with no further information about the device or test procedure and asked to perform the test in front of a health staff observer. The observer used product-specific semi-structured questionnaires with an observation checklist of the HIVST process, a sheet for recording test results, and a post-test interview that explored

participant experiences with the device and IFU, preferences, and WTP for the product. The observer systematically provided post-test counseling to the study participants after they performed and read the result. All participants provided a 3mL venous blood sample for confirmatory testing and made an appointment to receive their test result after two days. Participants received standard post-test counseling and support.

Data analysis

Double data entry was administered to enter data from paper-based questionnaires, using the KoboToolbox application and EpiData version 3.1. Data were converted to SPSS software version 22.0 for analysis, and they were analyzed using descriptive statistics and multivariable regression models (S1, S2, S3 and S4 Data). Variables found to be statistically significant (p -value <0.05) were included in the multivariable logistic regression. Multivariable logistic regression analysis was used to identify factors independently associated with successful completion of HIVST. The results of the analysis are presented as adjusted odds ratios (aOR) with 95% confidence intervals (CI) and interpreted as the odds of successful completion of the self-test among lay users who were exposed or not exposed to the associated factor. Variables included in the multivariable logistic regression analysis were age, sex, education, employment, ever HIV tested, and type of blood-based HIVST kit. The successful completion of self-testing was calculated as the percentage of participants that correctly performed key steps and obtained an interpretable result. The tests that failed to produce a control line were identified as INVALID and reported as failure.

Concordance of positive and negative HIVST results was calculated based on agreement rates of positive and negative self-test results interpreted by the study participants and by health staff observers. This analysis excluded incomplete self-tests, invalid test results interpreted by the health staff, and inconclusive (unsure) results interpreted by the study participants (using a 2x2 table).

Sensitivity and specificity were analyzed to measure the performance and accuracy of each HIVST kit. Sensitivity refers to the ability of the HIVST kits to accurately detect truly positive results, while specificity refers to the ability of the HIVST kits to correctly filter out truly negative results. Both outcomes improve as they approach 100%. This analysis excluded incomplete self-tests, invalid test results interpreted by the trained health staff, and inconclusive results interpreted by the study participants (using a 2x2 table) [49].

Results

Demographic and HIV testing history characteristics of the study participants

Among the 2,399 participants who agreed to HIVST, two-thirds (64.7%) were male and most (62.1%) were aged 25–49 years, while one-third (34.8%) were aged 18–24 years, and half (53.5%) had a higher education level. Most participants (69.8%) were employed or self-employed, while 26.2% were students, and 4.1% were unemployed, retired, or doing housework. About one-third (35.6%) had never tested for HIV, while 64.3% had tested previously (Table 1).

Acceptability of blood-based HIV self-tests

Of 2,404 eligible clients, 2,399 (99.8%) agreed to perform a blood-based HIV self-test, and all received confirmatory and ELISA tests (Fig 1).

Table 1. Demographic and HIV testing history characteristics of study participants by blood-based HIVST device.

| Characteristic | INSTI | SURE CHECK | BioSURE | CheckNOW | Total |
|----------------------------------|------------|------------|------------|------------|-------------|
| | n = 600 | n = 600 | n = 600 | n = 599 | n = 2,399 |
| | n (%) | n (%) | n (%) | n (%) | n (%) |
| Sex | | | | | |
| Male | 404 (67.3) | 383 (63.8) | 378 (63) | 386 (64.4) | 1551 (64.7) |
| Female | 196 (32.7) | 217 (36.2) | 222 (37) | 213 (35.6) | 848 (35.3) |
| Age in years (median) | 29 | 27 | 25 | 27 | 27 |
| 18–24 | 161 (26.8) | 177 (29.5) | 299 (49.8) | 198 (33.1) | 835 (34.8) |
| 25–49 | 416 (69.3) | 410 (68.3) | 287 (47.8) | 376 (62.8) | 1489 (62.1) |
| 50+ | 23 (3.8) | 13 (2.2) | 14 (2.3) | 25 (4.1) | 75 (3.1) |
| Education | | | | | |
| Primary school or lower | 17 (2.8) | 15 (2.5) | 7 (1.2) | 1 (0.1) | 40 (1.7) |
| Secondary school | 91 (15.2) | 77 (12.9) | 56 (9.3) | 43 (7.2) | 267 (11.2) |
| High school | 225 (37.5) | 185 (30.9) | 146 (24.3) | 251 (41.9) | 807 (33.6) |
| Higher education | 267 (44.5) | 321 (53.7) | 391 (65.2) | 304 (50.8) | 1283 (53.5) |
| Employment status | | | | | |
| Employed | 288 (48) | 280 (46.8) | 195 (32.5) | 229 (38.2) | 992 (41.4) |
| Freelance/self-employed | 210 (35) | 165 (27.6) | 119 (19.8) | 187 (31.2) | 681 (28.4) |
| Student | 68 (11.3) | 123 (20.6) | 264 (44.0) | 172 (28.7) | 627 (26.2) |
| Unemployed / retired / housework | 34 (5.7) | 30 (5) | 22 (3.7) | 11 (1.9) | 97 (4.1) |
| Ever been HIV tested | | | | | |
| Yes | 357 (59.5) | 315 (52.5) | 450 (75) | 421 (70.3) | 1543 (64.3) |
| No (first-time tester) | 243 (40.5) | 283 (47.2) | 150 (25) | 178 (29.7) | 854 (35.6) |
| Not sure | | 2 (0.3) | | | 2 (0.1) |

<https://doi.org/10.1371/journal.pgph.0001438.t001>

After performing the self-test, nearly all (94.4%) participants desired to use the test in the future, and 93.9% were willing to recommend the test (Table 2). About half (58.8%) preferred using the self-test at a clinic, while others preferred to use it at home (25.8%) or either at home or at a clinic (15.4%). The maximum median price of a blood-based HIVST kit that participants were WTP was \$US4.3 (95% CI: US\$4.6–\$5.3).

Fig 2 shows the declining trend of WTP for HIVST against increased price points. The vast majority (94.1%) of participants accepted the HIVST price that is equal to the price currently charged at public health facilities in Vietnam (i.e., \$ 2.6) and 69.6% were WTP at \$3.9, while only 37.2% accepted the price of \$5.2.

Feasibility of the blood-based HIV self-tests

Among 2,399 participants performing HIVST, the majority (90.8%) successfully completed the self-test or correctly performed all steps to obtain an interpretable result, whereas 9.2% failed to complete at least one critical step of the IFU that resulted in an uninterpretable result (Table 3). Common errors included using the lancet incorrectly to obtain the blood sample, particularly with INSTI and BioSURE (10.8% and 7.5%, respectively), or incorrectly transferring the specimen into the test (e.g., poor adherence to instructions to “Push hard through the foil cap until fully seated in the buffer cap”) with SURE CHECK (4.8%). Two-thirds (71.8%) could perform all steps of the IFU without hesitation, while 28.2% showed some hesitation in one or more steps. Most (63.1%) participants could perform the self-test without asking for

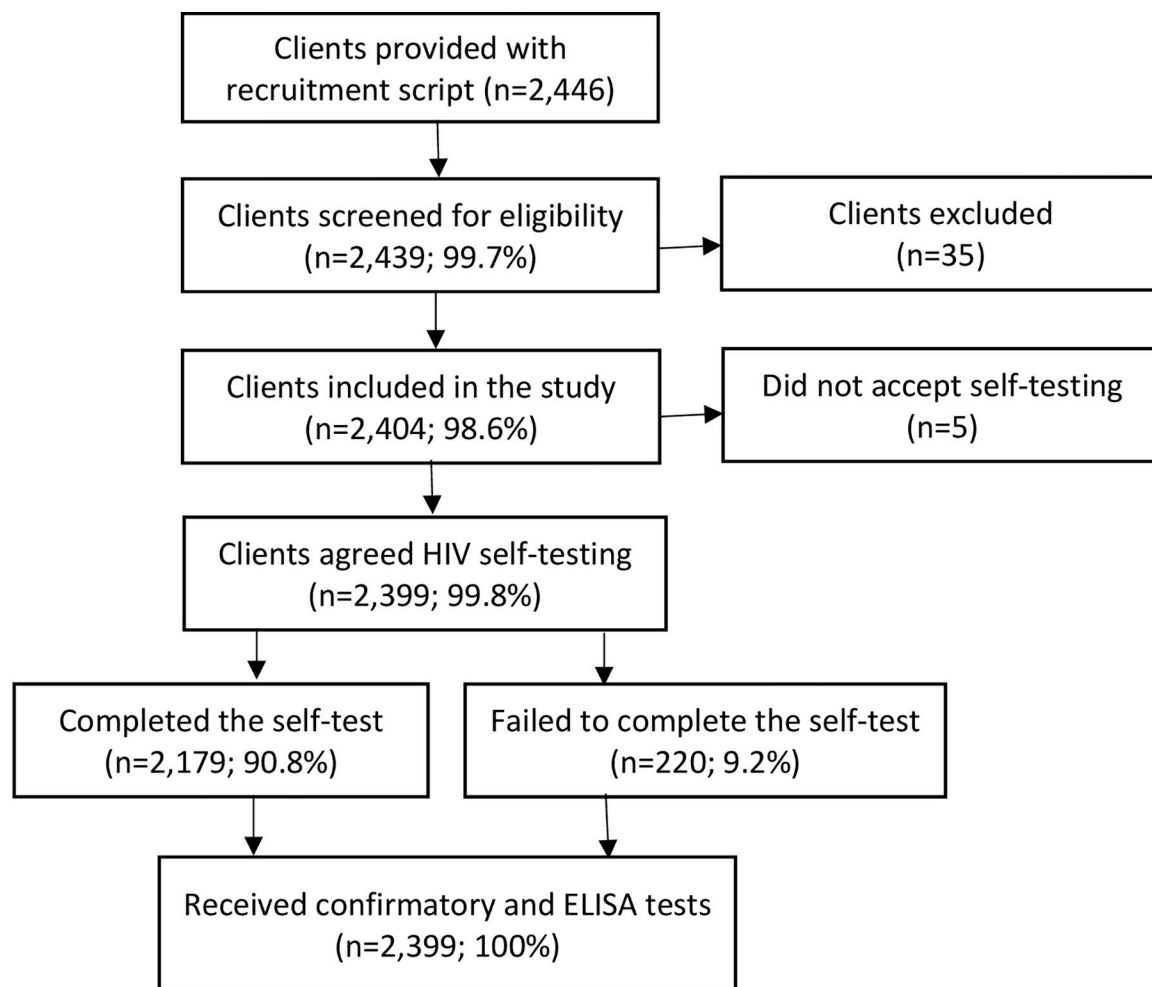


Fig 1. Enrollment of study participants.

<https://doi.org/10.1371/journal.pgph.0001438.g001>

any help, while 36.9% asked for help from the observer. The great majority (93%) of participants felt confident to perform the self-test (Table 3).

The multivariable logistic regression analysis (Table 4) identified a statistically significant association between successful completion of the self-test and higher education level (aOR = 1.85; 95% CI: 1.32–2.61). The multivariable analysis also confirmed a significant inverse association between successful completion of the self-test and self-testing with SURE CHECK (aOR = 0.21; 95% CI: 0.12–0.37), INSTI (aOR = 0.23; 95% CI: 0.13–0.39), or BioSURE (aOR = 0.29; 95% CI: 0.17–0.51), and being unemployed, retired, or doing housework (aOR = 0.45; 95% CI: 0.25–0.82).

Only participants who completed the self-test (2,179; 90.8%) were included in the agreement calculation for the test results interpreted between self-testers and health staff; 220 participants who failed to complete the self-test were excluded from this calculation. Overall, participants could correctly interpret positive/reactive and negative/nonreactive HIVST results at 98.1% and 99.9%, respectively, compared to the interpretation by trained health staff (Table 5). Agreement was reported at 100% for BioSURE and CheckNOW, while it was slightly lower for SURE CHECK (99.6%) and INSTI (99.1%).

Table 2. Acceptability, preference, and willingness to pay by blood-based HIV self-test device.

| Characteristic | INSTI | SURE CHECK | BioSURE | CheckNOW | Total |
|---|---------------------|---------------------|---------------------|-------------------|---------------------|
| | n = 600 | n = 600 | n = 600 | n = 599 | n = 2,399 |
| | n (%) | n (%) | n (%) | n (%) | n (%) |
| Recommendation the test to a friend or sexual partner | | | | | |
| Yes | 563 (94.1%) | 526 (88.1%) | 574 (95.7%) | 586 (97.8%) | 2,249 (93.9%) |
| No | 24 (4.0%) | 65 (10.9%) | 11 (1.8%) | 6 (1.0%) | 106 (4.4%) |
| Do not know | 11 (1.8%) | 6 (1.0%) | 15 (2.5%) | 7 (1.2%) | 39 (1.6%) |
| Desire to use the test in the future | | | | | |
| Yes | 561 (94.6%) | 543 (91.1%) | 559 (93.8%) | 588 (98.3%) | 2,251 (94.4%) |
| No | 25 (4.2%) | 38 (6.4%) | 12 (2.0%) | 3 (0.5%) | 78 (3.3%) |
| Do not know | 7 (1.2%) | 15 (2.5%) | 25 (4.2%) | 7 (1.2%) | 54 (2.3%) |
| Preference for use of the self-test | | | | | |
| At home | 129 (21.6%) | 313 (52.3%) | 106 (17.7%) | 70 (11.7%) | 618 (25.8%) |
| At a clinic | 325 (54.3%) | 193 (32.2%) | 429 (71.5%) | 461 (77.0%) | 1,408 (58.8%) |
| Either | 144 (24.1%) | 93 (15.5%) | 65 (10.8%) | 68 (11.3%) | 370 (15.4%) |
| Willingness to pay for HIVST | | | | | |
| Maximum median price in VND (\$) | 110K VND (\$4.8) | 100K VND (\$4.3) | 100K VND (\$4.3) | 90K VND (\$3.9) | 100K VND (\$4.3) |
| Maximum mean price 95% CI in VND (\$) | \$5.8 (\$5.2–\$6.4) | \$5.5 (\$5.1–\$5.9) | \$4.6 (\$4.3–\$4.9) | \$3.8 (\$3.6–\$4) | \$4.9 (\$4.6–\$5.3) |

Exchange rate: US\$1 = 23,000VND; VND, Vietnamese Dong. n, sample size and subsample size. HIVST, HIV self-test.

<https://doi.org/10.1371/journal.pgph.0001438.t002>

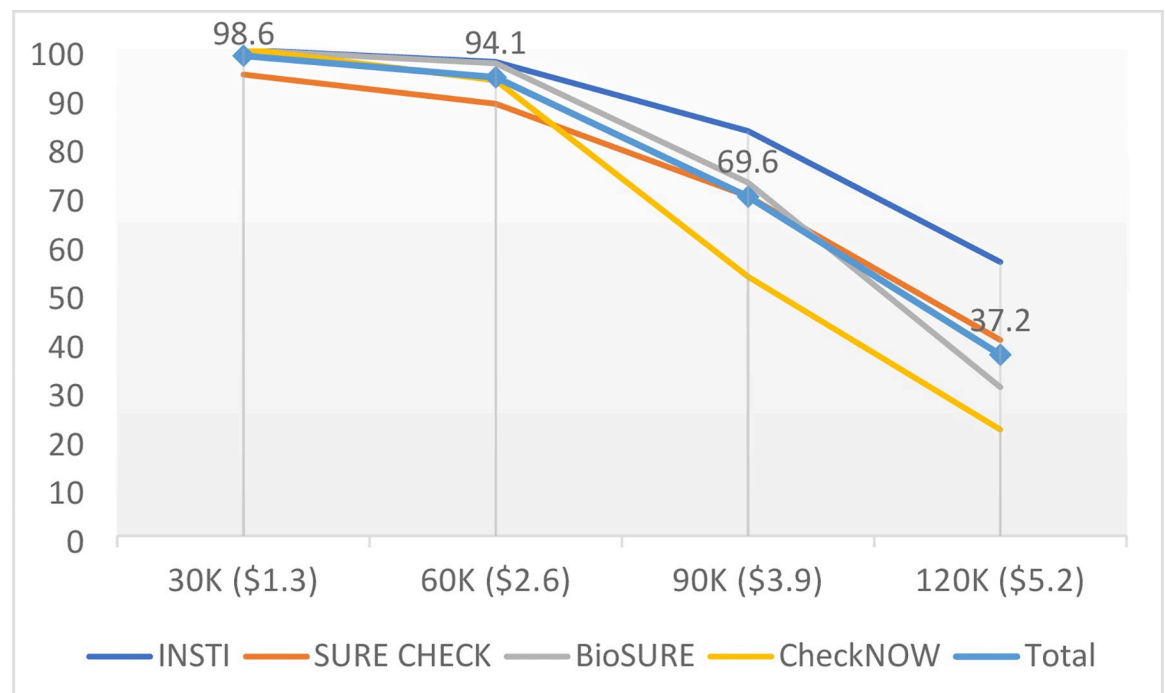


Fig 2. Willingness to pay by blood-based HIV self-test type (%).

<https://doi.org/10.1371/journal.pgph.0001438.g002>

Table 3. Ability to perform the blood-based HIV self-test, following the IFU.

| Characteristic | INSTI | SURE CHECK | BioSURE | CheckNOW | Total |
|---|------------|------------|------------|------------|--------------|
| | n = 600 | n = 600 | n = 600 | n = 599 | n = 2,399 |
| | n (%) | n (%) | n (%) | n (%) | n (%) |
| Successful completion of the self-test | | | | | |
| Completed | 522 (87) | 526 (87.7) | 550 (91.7) | 581 (97) | 2,179 (90.8) |
| Failed to complete | 78 (13) | 74 (12.3) | 50 (8.3) | 18 (3) | 220 (9.2) |
| Common mistakes in steps of the IFU | | | | | |
| Preparing the device | 2 (0.3) | 2 (0.3) | 3 (0.5) | 0 | 7 (0.3) |
| Obtaining the blood sample | 65 (10.8) | 43 (7.2) | 45 (7.5) | 17 (2.8) | 170 (7.1) |
| Transferring the specimen | 11 (1.8) | 29 (4.8) | 2 (0.3) | 1 (0.2) | 43 (1.8) |
| Hesitance in any step | | | | | |
| No | 409 (68.4) | 338 (56.9) | 404 (67.3) | 565 (94.3) | 1,716 (71.8) |
| Yes | 189 (31.5) | 256 (42.7) | 196 (32.7) | 34 (5.7) | 675 (28.2) |
| Asking for any help | | | | | |
| No | 371 (62.2) | 326 (54.5) | 363 (60.5) | 452 (75.5) | 1,512 (63.1) |
| Yes | 227 (37.8) | 272 (45.5) | 237 (39.5) | 147 (24.5) | 883 (36.9) |
| Perceived confidence by the self-tester | | | | | |
| No | 17 (2.8) | 31 (5.2) | 10 (1.7) | 9 (1.5) | 67 (2.8) |
| Yes | 551 (91.8) | 526 (87.7) | 578 (96.3) | 575 (96) | 2,230 (93) |
| Not sure | 32 (0.1) | 43 (7.2) | 12 (2.0) | 15 (2.5) | 102 (4.3) |

<https://doi.org/10.1371/journal.pgph.0001438.t003>

Accuracy of the blood-based HIV self-tests

Only participants who successfully achieved a self-test result on their own (2,080, 95.5%) were included in the performance calculation for sensitivity and specificity; 99 participants (i.e., 76 invalid, 6 inconclusive, and 17 indetermined [EIA] test results) were excluded from the calculation of HIVST performance. There were 162 (7.8%) true positive HIVST results (positive for both HIVST and EIA), 2 (0.1%) false positive results (positive for HIVST, negative for EIA), 1,910 (91.8%) true negative results (negative for both HIVST and EIA), and 6 (0.3%) false negative results (negative for HIVST, positive for EIA). This resulted in an average sensitivity of 96.4% (95% CI: 93.62–99.23) and a specificity of 99.9% (95% CI: 99.75–100), while also diagnosing 168 (8.1%) HIV-positive (sum of the true positives and false negatives) cases from the study population (Table 6).

Discussion

The HIV epidemic in Vietnam is concentrated among key populations, such as PWID, FSW, MSM, and transgender women. While HIV prevalence among PWID and FSW has declined, it has rapidly increased among MSM and transgender women in the last decade. The government of Vietnam has committed to achieving UNAIDS 95-95-95 goals and ending AIDS by 2030. HIV testing innovations, i.e., lay provider testing and self-testing, have been implemented in Vietnam since 2015 and 2016, respectively, with the aim of increasing access among unreached people. Evidence in Vietnam shows that these testing innovations are effective in reaching undiagnosed people and first-time testers or those who may not otherwise test or come to health facilities [50,51].

Our aim was to assess whether blood-based HIVST kits were acceptable, feasible, and accurate in the hands of unassisted lay users in the low HIV prevalence setting of Vietnam. Like other studies conducted in Peru, Brazil, Democratic Republic of the Congo (DRC), Thailand,

Table 4. Factors associated with the successful completion of the self-test.

| Multivariable analysis | Completed the self-test | | Univariable analysis | | Multivariable analysis | |
|--------------------------------|-------------------------|---------|----------------------|---------|------------------------|---------|
| | No (%) | Yes (%) | OR (95% CI) | P-value | aOR (95% CI) | P-value |
| Age | | | | | | |
| Above 29 years | 12.1 | 87.9 | 1 | | 1 | |
| 29 years or less | 7.4 | 92.6 | 1.7 (1.3–2.3) | 0.00*** | 1.3 (0.97–1.84) | 0.07 |
| Sex | | | | | | |
| Male | 8.9 | 91.1 | 1 | | 1 | |
| Female | 9.7 | 90.3 | 0.9 (0.7–1.2) | 0.5 | 1.13 (0.83–1.56) | 0.43 |
| Education level | | | | | | |
| High school or less | 13.0 | 87.0 | 1 | | 1 | |
| Higher education | 5.9 | 94.2 | 2.4 (1.8–3.2) | 0.00*** | 1.85 (1.32–2.61) | 0.00*** |
| Ever been HIV tested | | | | | | |
| Yes | 8.4 | 91.6 | 1 | | 1 | |
| No (first-time tester) | 9.6 | 90.4 | 0.9 (0.6–1.2) | 0.35 | 0.76 (0.56–1.03) | 0.08 |
| HIVST kit | | | | | | |
| CheckNOW | 3.0 | 97.0 | 1 | | 1 | |
| SURE CHECK | 12.3 | 87.7 | 0.22 (0.13–0.37) | 0.00*** | 0.21 (0.12–0.37) | 0.00*** |
| INSTI | 13.0 | 87.0 | 0.21 (0.12–0.35) | 0.00*** | 0.23 (0.13–0.39) | 0.00*** |
| BioSURE | 8.3 | 91.7 | 0.34 (0.19–0.6) | 0.00*** | 0.29 (0.17–0.51) | 0.00*** |
| Employment | | | | | | |
| Employed | 7.6 | 92.4 | 1 | | 1 | |
| Freelance, self-employed | 12.9 | 87.1 | 0.55 (0.4–0.8) | 0.00*** | 0.7 (0.5–1) | 0.051 |
| Student | 5.6 | 94.4 | 1.38 (0.9–2.1) | 0.125 | 1.06 (0.67–1.68) | 0.81 |
| Unemployed, retired, housework | 21.7 | 78.4 | 0.3 (0.2–0.5) | 0.00*** | 0.45 (0.25–0.82) | 0.01** |
| Eyesight impairment | | | | | | |
| Yes | 6.9 | 93.1 | 1 | | 1 | |
| No | 10.5 | 89.5 | 0.63 (0.5–0.9) | 0.01** | 0.85 (0.62–1.2) | 0.35 |

Logistic regression

*p < 0.05

**p < 0.01

***p < 0.001. CI, confidence interval. OR, odds ratio; aOR, adjusted odds ratio. HIVST, HIV self-test.

<https://doi.org/10.1371/journal.pgph.0001438.t004>

Table 5. Agreement between participant-interpreted HIVST result and health staff–interpreted result.

| Characteristic | INSTI | SURE CHECK | BioSURE | CheckNOW | Total |
|----------------------------------|---------|------------|---------|----------|-----------|
| | n = 522 | n = 526 | n = 550 | n = 581 | n = 2,179 |
| HIVST results interpreted | | | | | |
| Concordant positive | 54 | 42 | 26 | 41 | 163 |
| Concordant negative | 408 | 475 | 488 | 534 | 1,905 |
| Discordant positive | 1 | 0 | 0 | 0 | 1 |
| Discordant negative | 3 | 1 | 0 | 0 | 4 |
| Invalid, inconclusive | 56 | 8 | 36 | 6 | 106 |
| Calculation | | | | | |
| Positive percent agreement | 94.7% | 97.7% | 100% | 100% | 98.1% |
| Negative percent agreement | 99.7% | 100% | 100% | 100% | 99.9% |
| Total percent agreement | 99.1% | 99.6% | 100% | 100% | 99.7% |

<https://doi.org/10.1371/journal.pgph.0001438.t005>

Table 6. Performance of HIV self-tests compared to the ‘gold standard’ fourth generation ELISA test.

| HIVST performance | INSTI | SURE CHECK | BioSURE | CheckNOW | Total |
|-------------------------|-------------------------|-----------------------|-----------------------|-----------------------|-------------------------|
| | n = 522 | n = 526 | n = 550 | n = 581 | n = 2,179 |
| True positive | 54 (10.3%) | 42 (8.0%) | 26 (4.7%) | 40 (6.9%) | 162 (7.4%) |
| True negative | 422 (80.8%) | 468 (89.0%) | 486 (88.4%) | 534 (91.9%) | 1910 (87.7%) |
| False positive | 1 (0.2%) | 0 (0.0%) | 0 (0.0%) | 1 (0.2%) | 2 (0.1%) |
| False negative | 4 (0.8%) | 1 (0.2%) | 1 (0.2%) | 0 (0.0%) | 6 (0.3%) |
| Invalid | 36 (6.9%) | 7 (1.3%) | 27 (4.9%) | 6 (1.0%) | 76 (3.5%) |
| Inconclusive | 5 (1.0%) | 1 (0.2%) | 0 (0.0%) | 0 (0%) | 6 (0.3%) |
| In-determined | 0 (0.0%) | 7 (1.3%) | 10 (1.8%) | 7 (1.2%) | 17 (0.8%) |
| Calculation | | | | | |
| Sensitivity (95% CI) | 93.10% (86.58–99.62) | 97.67% (93.17–100) | 96.30% (89.17–100) | 100% (100–100) | 96.43% (93.62–99.23) |
| Specificity (95% CI) | 99.76% (99.30–100) | 100% (100–100) | 100% (100–100) | 99.81% (99.45–100) | 99.90% (99.75–100) |
| Accuracy (95% CI) | 98.96% (98.05–99.87) | 99.80% (99.42–100) | 99.80% (99.42–100) | 99.80% (99.49–100) | 99.62% (99.35–99.88) |

n, sample size and subsample size. CI, confident interval. HIVST, HIV self-test.

<https://doi.org/10.1371/journal.pgph.0001438.t006>

and Kenya [7,12,52–54], we found the blood-based HIVST was highly acceptable and in demand, and those who used an HIVST product desired to use it again in the future and/or were willing to recommend the test to a friend or sexual partner. Although WTP for the blood-based HIVST kits studied was relatively high (median price of US\$4.3), this preferred price is still lower than the average private-sector price in LMICs (US\$7–\$12) [34]. This suggests that catalytic market interventions like those implemented by the Gates Foundation and Unitaid with HIVST manufacturers to offer lower-cost HIVST kits (US\$2 per test) in high-HIV-burden LMIC settings should be continued to facilitate scale-up of HIVST, increase purchase volumes, and eventually lower prices [34,55,56].

There has been concern over the usability of blood-based HIVST in lay users because of its more invasive and painful finger prick compared to oral fluid-based HIVST [17]. Our findings confirmed that performing blood-based HIVST without assistance was highly feasible, and successful completion of the self-test was significantly associated with higher education level. This finding is similar to previous studies of blood-based HIVST kits conducted in DRC, Thailand, Central African Republic, South Africa, and Canada [25,32,38,53,54,57]. Despite the feasibility of blood-based HIVST, the study observed errors in obtaining the blood sample or transferring the specimen to the test, suggesting the need for modification of IFU materials to improve usability. This validated similar findings from previous studies where most errors occurred during the specimen collection stage among finger-prick HIVST users [19,26]. We also found that correct interpretation of blood-based HIVST results by lay users was as high as by trained health staff. This suggests that INSTI, SURE CHECK, BioSURE, and CheckNOW are likely appropriate for use in the untrained and unsupervised general or key population.

Accuracy of HIVST performed by lay users is the most important concern [6,7,54]. Like previous studies in South Africa and Canada [33,57], we found that the sensitivity of all four blood-based HIVST devices evaluated in this study was high, ranging from 93.1% to 100%, and the specificity ranged from 99.76% to 100%. These results are compatible with the accuracy reported by the respective products’ manufacturers. The high sensitivity and specificity of HIVST devices in this study suggested that blood-based HIVST is an excellent tool for people to self-screen for HIV. Each batch of devices was manufactured under ISO 14385 standards

required for the design and manufacture of medical devices and each HIVST kit included IFU with minimal language and simple pictorial instructions. At the time of this publication submission, all four devices in this assessment (INSTI, SURE CHECK, BioSURE, and Check-NOW) had been WHO prequalified, using data generated in this study and the parallel study in South Africa [33]. Despite the high sensitivity and specificity, there were several user errors (notably with INSTI, BioSURE, and SURE CHECK), highlighting areas for improvement.

Where blood-based HIVST products have been registered and made available as part of the product mix in LMICs, there has been greater versatility in the face of COVID-19. Countries like Vietnam, Ukraine, Uganda, DRC, and Kenya, that already had an HIVST program in place, were able to pivot rapidly and increase delivery of HIVST in lieu of facility or lay provider-based testing, to maintain continuity of care and essential prevention and treatment services [3,46]. HIVST has also played an important role with PrEP delivery during the COVID-19 pandemic, enabling telemedicine combined with home monitoring of HIV status using blood-based HIVST kits [1].

Limitations

This study has several limitations. A selection bias may have been created with convenience sampling. Those seeking an HIV test at the Pasteur Institute were able to pay for their test and therefore the WTP in this study may not be representative of the entire HIV testing population. Duplication of recruitments may happen when the assessment was conducted using multiple devices in a series. We employed the fingerprint scanning system to eliminate the duplication of participants. An observation bias may have been present, as the study was conducted under observation in a clinical setting. The usability of blood-based HIVST at home or outside clinical settings may be different. For data collection, there was no standardized usability test for HIVST, so the product-specific questionnaire was developed internally and used to assess usability. This questionnaire only allowed for each device to be assessed independently. No direct comparisons between products could be assessed. The WHO prequalification only requires independent data on usability and does not require any direct comparisons between products; however, we are developing a standardized tool as a separate project because comparisons would be beneficial as more HIV self-tests reach the market.

Conclusions

Our findings confirm that blood-based HIV self-testing is highly acceptable, feasible, and accurate. These findings are critical to inform the scale-up of blood-based HIVST in addition to oral fluid-based HIVST to offer greater product choice to those that seek testing, and therefore increase HIV testing uptake and access to essential HIV prevention (like PrEP) and treatment services. The COVID-19 pandemic has made increased access to a range of affordable blood-based and oral fluid-based HIVST more important than ever. As lockdowns are lifted and populations are increasingly able to safely seek in-person care, HIVST is a critical tool for accelerating catch-up of HIV testing among the many people that have gone without it.

Supporting information

S1 Text. Questionnaire for INSTI HIVST.
(DOCX)

S2 Text. Questionnaire for SURE CHECK HIVST.
(DOCX)

S3 Text. Questionnaire for BioSURE HIVST.
(DOCX)

S4 Text. Questionnaire for CheckNOW HIVST.
(DOCX)

S1 Data. Dataset of INSTI HIVST.
(SAV)

S2 Data. Dataset of SURE CHECK HIVST.
(SAV)

S3 Data. Dataset of BioSURE HIVST.
(SAV)

S4 Data. Dataset of CheckNOW HIVST.
(SAV)

Acknowledgments

We thank all the study participants for their contributions. We are grateful to the Pasteur Institute in Ho Chi Minh City, Vietnam, for its collaboration and commitment in implementing the study. A thank you to Gillian Anderson and Zoe Humeau for their review and edits to improve this manuscript.

Author Contributions

Conceptualization: Bao Vu Ngoc, Mohammed Majam, Kimberly Green.

Data curation: Bao Vu Ngoc, Minh Tran Hung, Diep Bui Ngoc.

Formal analysis: Bao Vu Ngoc, Minh Tran Hung, Diep Bui Ngoc.

Funding acquisition: Mohammed Majam, Kimberly Green.

Investigation: Ton Tran, Minh Tran Hung, Anh Luong Que, Chuong Hoang Le Duy.

Methodology: Bao Vu Ngoc, Mohammed Majam, Ton Tran, Minh Tran Hung.

Project administration: Bao Vu Ngoc, Ton Tran, Anh Luong Que, Chuong Hoang Le Duy.

Software: Diep Bui Ngoc.

Supervision: Bao Vu Ngoc, Ton Tran, Minh Tran Hung, Anh Luong Que, Diep Bui Ngoc, Chuong Hoang Le Duy.

Validation: Bao Vu Ngoc, Minh Tran Hung, Anh Luong Que, Diep Bui Ngoc.

Visualization: Bao Vu Ngoc.

Writing – original draft: Bao Vu Ngoc.

Writing – review & editing: Bao Vu Ngoc, Kimberly Green.

References

1. World Health Organization. Consolidated guidelines on HIV prevention, testing, treatment, service delivery and monitoring: recommendations for public health approach. Geneva: WHO; 2021 July 16. Available from <https://www.who.int/publications/i/item/9789240031593>.

2. World Health Organization and Human Reproduction Programme. WHO guideline on self-care interventions for health and well-being. Geneva: WHO; 2021. Available from <https://apps.who.int/iris/bitstream/handle/10665/342741/9789240030909-eng.pdf>.
3. Unitaid. Considerations for HIV Self-Testing in the context of the COVID-19 Pandemic and its Response: An Operational Update. 2021. Available from: <https://www.path.org/resources/considerations-hiv-self-testing-context-covid-19-pandemic-and-its-response-operational-update/>.
4. Choko AT, Desmond N, Webb EL, Chavula K, Napierala-Mavedzenge S, Gaydos CA, et al. The uptake and accuracy of oral kits for HIV self-testing in high HIV prevalence setting: a cross-sectional feasibility study in Blantyre, Malawi. *PLoS Med*. 2011; 8(10):1–11. <https://doi.org/10.1371/journal.pmed.1001102> PMID: 21990966
5. Choko AT, MacPherson P, Webb EL, Willey BA, Feasy H, Sambakunsi R, et al. Uptake, Accuracy, Safety, and Linkage into Care over Two Years of Promoting Annual Self-Testing for HIV in Blantyre, Malawi: A Community-Based Prospective Study. *PLoS Med*. 2015; 12(9):e1001873. <https://doi.org/10.1371/journal.pmed.1001873> PMID: 26348035
6. Lee VJ, Tan SC, Earnest A, Seong PS, Tan HH, Leo YS. User acceptability and feasibility of self-testing with HIV rapid tests. *J Acquir Immune Defic Syndr [Internet]*. 2007; 45(4):449–453. <https://doi.org/10.1097/QAI.0b013e318095a3f3> PMID: 17554213
7. Volk JE, Lippman SA, Grinsztejn B, Lama JR, Fernandes NM, Gonzales P, et al. Acceptability and feasibility of HIV self-testing among men who have sex with men in Peru and Brazil. *Int J STD AIDS*. 2016 Jun; 27(7):531–536. <https://doi.org/10.1177/0956462415586676> PMID: 25971262
8. Tao J, Li M, Qian H-Z, Wang L-J, Zhang Z, Ding H-F, et al. Home-based HIV testing for men who have sex with men in China: a novel community-based partnership to complement government programs. *PLoS One*. 2014; 9(7):e102812. <https://doi.org/10.1371/journal.pone.0102812> PMID: 25051160
9. Asimwe S, Oloya J, Song X, Whalen CC. Accuracy of Un-supervised Versus Provider-Supervised Self-administered HIV Testing in Uganda: A Randomized Implementation Trial. *AIDS Behav*. 2014; 18(12):2477–2484. <https://doi.org/10.1007/s10461-014-0765-4> PMID: 24691923
10. Kurth AE, Cleland CM, Chhun N, Sidle JE, Were E, Naanyu V, et al. Accuracy and Acceptability of Oral Fluid HIV Self-Testing in a General Adult Population in Kenya. *AIDS Behav*. 2016; 20(4):870–879. <https://doi.org/10.1007/s10461-015-1213-9> PMID: 26438487
11. Tonen-Wolyec S, Sarassoro A, Muwonga Masidi J, Twite Banza E, Nsiku Dikumbwa G, Maseke Matondo DM, et al. Field evaluation of capillary blood and oral-fluid HIV self-tests in the Democratic Republic of the Congo. *PLoS One*. 2020; 15(10):e0239607. <https://doi.org/10.1371/journal.pone.0239607> PMID: 33017442
12. Bwana P, Ochieng L, Mwau M. Performance and usability evaluation of the INSTI HIV self-test in Kenya for qualitative detection of antibodies to HIV. *PLoS One*. 2018 Sep 13; 13(9):e0202491. <https://doi.org/10.1371/journal.pone.0202491> PMID: 30212525
13. Neuman M, Mwinga A, Kapaku K, Sigande L, Gotsche C, Taegtmeier M, et al. Sensitivity and specificity of OraQuick HIV self-test compared to a 4th generation laboratory reference standard algorithm in urban and rural Zambia. *BMC Infect Dis*. 2022; 22:494. <https://doi.org/10.1186/s12879-022-07457-5> PMID: 35614397
14. Lippman SA, Moran L, Sevelius J, Castillo LS, Ventura A, Treves-Kagan S, et al. Acceptability and Feasibility of HIV Self-Testing Among Transgender Women in San Francisco: A Mixed Methods Pilot Study. *AIDS Behav*. 2016; 20(4):928–938. <https://doi.org/10.1007/s10461-015-1236-2> PMID: 26511864
15. van Rooyen H, Tulloch O, Mukoma W, Makusha T, Chepuka L, Knight LC, et al. What are the constraints and opportunities for HIVST scale-up in Africa? Evidence from Kenya, Malawi and South Africa. *J Int AIDS Soc*. 2015; 18:19445. <http://www.jiasociety.org/index.php/jias/article/view/19445> | <http://dx.doi.org/10.7448/IAS.18.1.19445> PMID: 25797344
16. Kumwenda M, Munthali A, Phiri M, Mwale D, Gutteberg T, MacPherson E, et al. Factors Shaping Initial Decision-Making to Self-test Amongst Cohabiting Couples in Urban Blantyre, Malawi. *AIDS Behav*. 2014; 18:S396–S404; <https://doi.org/10.1007/s10461-014-0817-9> PMID: 24929834
17. Peck RB, Lim JM, Van Rooyen H, Mukoma W, Chepuka L, Bansil P, et al. What should the ideal HIV self-test look like? A usability study of test prototypes in unsupervised HIV self-testing in Kenya, Malawi, and South Africa. *AIDS Behav*. 2014; 18(Suppl 4):S422–S432.
18. Pant Pai N, Behlim T, Abrahams L, Vadnais C, Shivkumar S, Pillay S, et al. Will an unsupervised self-testing strategy for HIV work in health care workers of South Africa? A cross sectional pilot feasibility study. *PLoS One*. 2013; 8(11):e79772. <https://doi.org/10.1371/journal.pone.0079772> PMID: 24312185
19. Pant Pai N, Bhargava M, Joseph L, Sharma J, Pillay S, Balram B, et al. Will an unsupervised self-testing strategy be feasible to operationalize in Canada? Results from a pilot study in students of a large

- Canadian university. *AIDS Res Treat*. 2014; 2014:1–8. <https://doi.org/10.1155/2014/747619> PMID: 24511392
20. Kalibala S, Tun W, Cherutich P, Nganga A, Oweya E, Oluoch P. Factors associated with acceptability of HIV self-testing among health care workers in Kenya. *AIDS Behav*. 2014; 18(Suppl 4):S405–S414. Available from: <http://www.ncbi.nlm.nih.gov/pubmed/24974123>. <https://doi.org/10.1007/s10461-014-0830-z> PMID: 24974123
21. Ng OT, Chow AL, Lee VJ, Chen MIC, Win MK, Tan HH, et al. Accuracy and User-Acceptability of HIV Self-Testing Using an Oral Fluid-Based HIV Rapid Test. *PLoS One*. 2012; 7(9):e45168. <https://doi.org/10.1371/journal.pone.0045168> PMID: 23028822
22. Gaydos CA, Hsieh YH, Harvey L, Burah A, Won H, Jett-Goheen M, et al. Will patients “opt in” to perform their own rapid HIV test in the emergency department? *Ann Emerg Med*. 2011; 58(1 Suppl 1):S74–S78. <https://doi.org/10.1016/j.annemergmed.2011.03.029> PMID: 21684413
23. Marley G, Kang D, Wilson EC, Huang T, Qian Y, Li X, et al. Introducing rapid oral-fluid HIV testing among high risk populations in Shandong, China: feasibility and challenges. *BMC Public Health*. 2014; 14(422):1–8. <https://doi.org/10.1186/1471-2458-14-422> PMID: 24884431
24. Lippman SA, Gilmore HJ, Lane T, Radebe O, Chen Y-H, Mlotshwa N, et al. Ability to use oral fluid and fingerstick HIV self-testing (HIVST) among South African MSM. *PLoS One*. 2018; 13(11):e0206849. <https://doi.org/10.1371/journal.pone.0206849> PMID: 30408055
25. Smith P, Wallace M, Bekker LG. Adolescents’ experience of a rapid HIV self-testing device in youth friendly clinic settings in Cape Town South Africa: a cross-sectional community-based usability study. *J Int AIDS Soc*. 2016; 19(1):21111. <http://www.jiasociety.org/index.php/jias/article/view/21111> | <http://dx.doi.org/10.7448/IAS.19.1.21111>. PMID: 28406597
26. Wei C, Yan L, Li J, Su X, Lippman S, Yan H. Which user errors matter during HIV self-testing? A qualitative participant observation study of men who have sex with men (MSM) in China. *BMC Public Health*. 2018; 18:1108. <https://doi.org/10.1186/s12889-018-6007-3> PMID: 30200905
27. de la Fuente L, Rosales-Statkus ME, Hoyos J, Pulido J, Santos S, Bravo MJ, et al. Are participants in a street-based HIV testing program able to perform their own rapid test and interpret the results? *PLoS One*. 2012; 7(10):1–10.
28. Ng OT, Chow AL, Lee VJ, Chen MIC, Win MK, Tan HH, et al. Accuracy and User-Acceptability of HIV Self-Testing Using an Oral Fluid-Based HIV Rapid Test. *PLoS One*. 2012; 7(9):e45168. <https://doi.org/10.1371/journal.pone.0045168> PMID: 23028822
29. Gaydos CA, Solis M, Hsieh YH, Jett-Goheen M, Nour S, Rothman RE. Use of tablet-based kiosks in the emergency department to guide patient HIV self-testing with a point-of-care oral fluid test. *Int J STD AIDS*. 2013; 24(9):716–21. <https://doi.org/10.1177/0956462413487321> PMID: 23970610
30. Nour S, Hsieh YH, Rothman RE, Jett-Goheen M, Langhorne O, Wu L, et al. Patients Can Accurately Perform Their Own Rapid HIV Point-of-Care Test in the Emergency Department. *Point Care*. 2012; 11(4):176–179. <https://doi.org/10.1097/POC.0b013e3182666eb7> PMID: 24031999
31. Majam M, Mazzola L, Rhagnath N, LallaEdward ST, Mahomed R, Venter WDF, et al. Usability assessment of seven HIV self-test devices conducted with lay-users in Johannesburg, South Africa. *PLoS One*. 2020; 15(1):e0227198. <https://doi.org/10.1371/journal.pone.0227198> PMID: 31935228
32. Gresenguet G, Longo DJ, Tonen-Wolyec S, Mbouma Bouassa RS, Bélec L. Acceptability and Usability Evaluation of Finger-Stick Whole Blood HIV Self-Test as An HIV Screening Tool Adapted to The General Public in The Central African Republic. *Open AIDS J*. 2017; 11:101–118. <https://doi.org/10.2174/1874613601711010101> PMID: 29290887
33. Majam M, Fischer AE, Rhagnath N, Msolomba V, Venter WD, Mazzola L, et al. Performance assessment of four HIV self-test devices in South Africa: A cross-sectional study. *S Afr J Sci*. 2021; 117(1/2). <https://doi.org/10.17159/sajs.2021/7738>.
34. Unitaid/WHO. HIV self-testing technology landscape: HIV rapid diagnostic tests for self-testing. 4th edition. Geneva: Unitaid; 2018 July. Available from <https://unitaid.org/assets/HIVST-landscape-report.pdf>.
35. Thirumurthy H, Masters SH, Agot K. Willingness to pay for HIV self-tests among women in Kenya: implications for subsidy and pricing policies. *J Acquir Immune Defic Syndr*. 2018 June 01; 78(2):e8–e11. <https://doi.org/10.1097/QAI.0000000000001659> PMID: 29767641
36. Ashburn K, Antelman G, N’Goran MK, Jahanpour O, Yemaneberhan A, Kouakou BN, et al. Willingness to use HIV self-test kits and willingness to pay among urban antenatal clients in Cote d’Ivoire and Tanzania: a cross-sectional study. *Trop Med and Int Health*. 2020; 25(9):1155–1165. <https://doi.org/10.1111/tmi.13456> PMID: 32609932
37. Pal K, Ngin C, Tuot S, Chhoun P, Ly C, Chhim S, et al. Acceptability Study on HIV Self-Testing among Transgender Women, Men Who Have Sex with Men, and Female Entertainment Workers in Cambodia: A Qualitative Analysis. *PLoS One*. 2016; 11(11):e0166129. <https://doi.org/10.1371/journal.pone.0166129> PMID: 27829064

38. Tonen-Wolyec S, Tshilumba CK, Batina-Agasa S, Djang'eing'a RM, Hayette MP, Bélec L. Comparison of practicability and effectiveness between unassisted HIV self-testing and directly assisted HIV self-testing in the Democratic Republic of the Congo: a randomized feasibility trial. *BMC Infect Dis*. 2020 Nov 11; 20(1):830. <https://doi.org/10.1186/s12879-020-05554-x> PMID: 33176700
39. Xun H, Kang D, Huang T, Qian Y, Li X, Wilson EC, et al. Factors associated with willingness to accept oral fluid HIV rapid testing among most-at-risk populations in China. *PLoS One*. 2013; 8(11):e80594. <https://doi.org/10.1371/journal.pone.0080594> PMID: 24260432
40. Piamonte SBH, Ditangco RA. Awareness and willingness to pay for HIV self-test among men who have sex with men from metro Manila, Philippines. *Malays J Pub Health Med*. 2020; 20(1):64–70.
41. Tun W, Vu L, Dirisu O, Sekoni A, Shoyemi E, Njab J, et al. Uptake of HIV self-testing and linkage to treatment among men who have sex with men (MSM) in Nigeria: A pilot programme using key opinion leaders to reach MSM. *J Int AIDS Soc*. 2018; 21(S5):e25124. <http://onlinelibrary.wiley.com/doi/10.1002/jia2.25124/full> | <https://doi.org/10.1002/jia2.25124> PMID: 30033680
42. Ortblad KF, Musoke DK, Ngabirano T, Nakitende A, Taasi G, Barresi LG, et al. HIV self-test performance among female sex workers in Kampala, Uganda: a cross-sectional study. *BMJ Open*. 2018; 8:e022652. <https://doi.org/10.1136/bmjopen-2018-022652> PMID: 30413504
43. Bao VN, Green K, Minh TH, Ha VS, Tu LN, Reddy CK. Are HIV-affected populations willing and able to pay for HIV prevention goods and services? Results from a cross-sectional study in Vietnam. Poster presented at the 21st International AIDS Conference; 2016 July 18–22; Durban, South Africa. Available from: <https://www.path.org/media-center/path-at-aids-2016/>.
44. Didier KE, Bitty-Anderson A, Fifonsi AGK, Ahuatchi PC, Serge PE. HIV self-testing: The key to unlock the first 90 in West and Central Africa. *Int J Infect Dis*. 2020; 95:162–166. <https://doi.org/10.1016/j.ijid.2020.02.016> PMID: 32070722
45. The Global Fund. Results report 2021. Available from: https://www.theglobalfund.org/media/11304/corporate_2021resultsreport_report_en.pdf.
46. Green K, Tham TT, Thanh LM, Huy VB, Thu NT, Bao VN, et al. The #Stayhome #Selftest campaign: Rapid pivot of HIV testing services to enable continuity of care in Hanoi, Vietnam, during the COVID-19 lockdown. OADLB01 oral abstract; late-breaker; 23rd International AIDS Conference; 2020 July 6–10; San Francisco, CA, USA (Virtual). Available from: <https://search.bvsalud.org/global-literature-on-novel-coronavirus-2019-ncov/resource/fr/covidwho-705405>.
47. Lee VJ, Tan SC, Earnest A, Seong PS, Tan HH, Leo YS. User acceptability and feasibility of self-testing with HIV rapid tests. *J Acquir Immune Defic Syndr*. 2007; 45(4):449–453. <https://doi.org/10.1097/QAI.0b013e318095a3f3> PMID: 17554213
48. World Health Organization. Technical specifications for WHO prequalification of Human Immunodeficiency Virus (HIV) rapid diagnostic tests for professional use and/or self-testing. Geneva: WHO; 2016. Available from <https://apps.who.int/iris/handle/10665/251857>.
49. Parikh R, Mathai A, Parikh S, Chandra Sekhar G, Thomas R. Understanding and using sensitivity, specificity and predictive values. *Indian J Ophthalmol*. 2008 Jan-Feb; 56(1):45–50. <https://doi.org/10.4103/0301-4738.37595> PMID: 18158403
50. Vu BN, Green KE, Thi Thu Phan H, Hung Tran M, Van Ngo H, Hai Vo S, et al. Lay provider HIV testing: A promising strategy to reach the undiagnosed key populations in Vietnam. *PLoS One*. 2018; 13(12):e0210063. <https://doi.org/10.1371/journal.pone.0210063> PMID: 30596777
51. Green KE, Vu BN, Phan HTT, Tran MH, Ngo HV, Vo SH, et al. From conventional to disruptive: upturning the HIV testing status quo among men who have sex with men in Vietnam. *J Int AIDS Soc*. 2018; 21(S5):e25127. <http://onlinelibrary.wiley.com/doi/10.1002/jia2.25127/full> | <https://doi.org/10.1002/jia2.25127>.
52. Magno L, Leal AF, Knauth D, Dourado I, Guimarães MDC, Santana EP, et al. Acceptability of HIV self-testing is low among men who have sex with men who have not tested for HIV: a study with respondent-driven sampling in Brazil. *BMC Infect Dis*. 2020; 20:865. <https://doi.org/10.1186/s12879-020-05589-0> PMID: 33213389
53. Tonen-Wolyec S, Batina-Agasa S, Muwonga J, Mboumba Bouassa RS, Kayembe Tshilumba C, Bélec L. Acceptability, feasibility, and individual preferences of blood-based HIV self-testing in a population-based sample of adolescents in Kisangani, Democratic Republic of the Congo. *PLoS One*. 2019; 14(7):e0218795. <https://doi.org/10.1371/journal.pone.0218795> PMID: 31260480
54. Phongphiew P, Songtaweasin WN, Paiboon N, Phiphatkhunarnon P, Srimuan P, Sowaprun T, et al. Acceptability of blood-based HIV self-testing among adolescents aged 15–19 years at risk of HIV acquisition in Bangkok. *Int J STD AIDS*. 2021; 32(10):927–932. <https://doi.org/10.1177/09564624211003742> PMID: 33890847
55. OraSure Technologies Inc. OraSure Technologies to Drive Accelerated Adoption of OraQuick HIV Self-Test. *Intrado GlobeNewswire*; 2017 June 27. Available from: <https://www.globenewswire.com/news->

[release/2017/06/27/1029393/0/en/OraSure-Technologies-to-Drive-Accelerated-Adoption-of-OraQuick-HIV-Self-Test.html](https://www.plos.org/news/2017/06/27/1029393/0/en/OraSure-Technologies-to-Drive-Accelerated-Adoption-of-OraQuick-HIV-Self-Test.html).

56. Unitaid. Access to HIV self-tests significantly expanded and costs halved thanks to Unitaid agreement. 28 April 2021. Press Release. Available from: <https://unitaid.org/news-blog/access-to-hiv-self-tests-significantly-expanded-and-costs-halved-thanks-to-unitaid-agreement/#en>.
57. Galli RA, Tian JMLH, Sumner-Williams M, McBain K, Stanizai E, Tharao W, et al. An observed, prospective field study to evaluate the performance and acceptance of a blood-based HIV self-test in Canada. BMC Public Health. 2021; 21:1421. <https://doi.org/10.1186/s12889-021-11418-z>. PMID: 34275450